
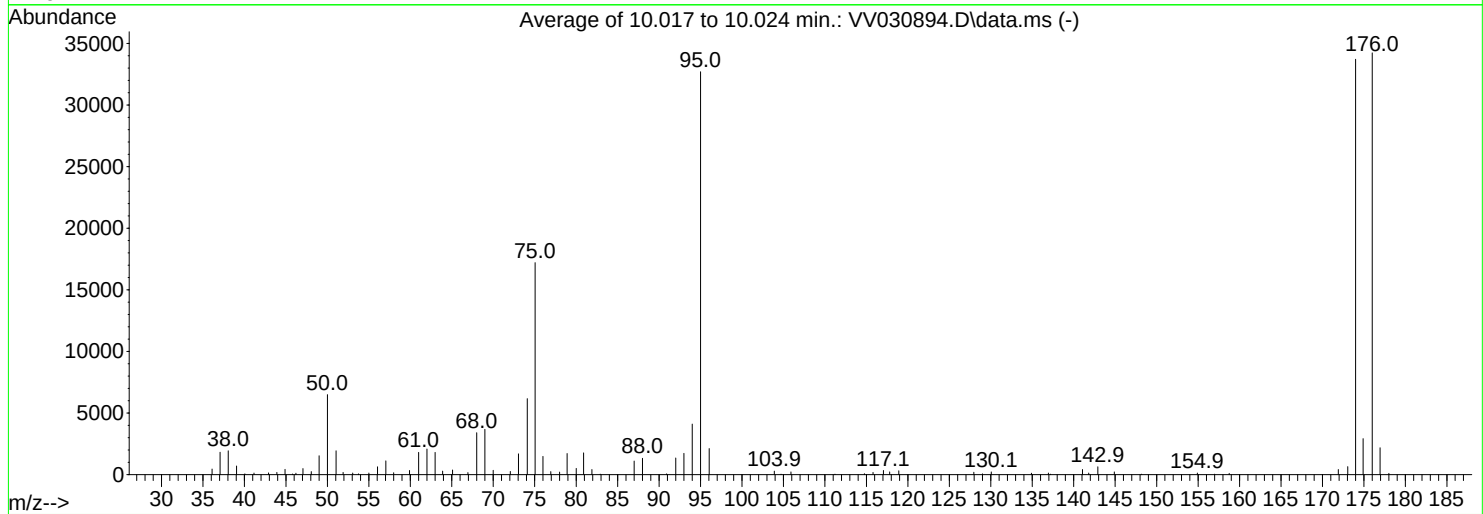


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042723\
Data File : VV030894.D
Acq On : 27 Apr 2023 09:23
Operator : SY/MD
Sample : BFB374
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB374

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Title : VOC Analysis
Last Update : Thu Apr 27 04:45:18 2023

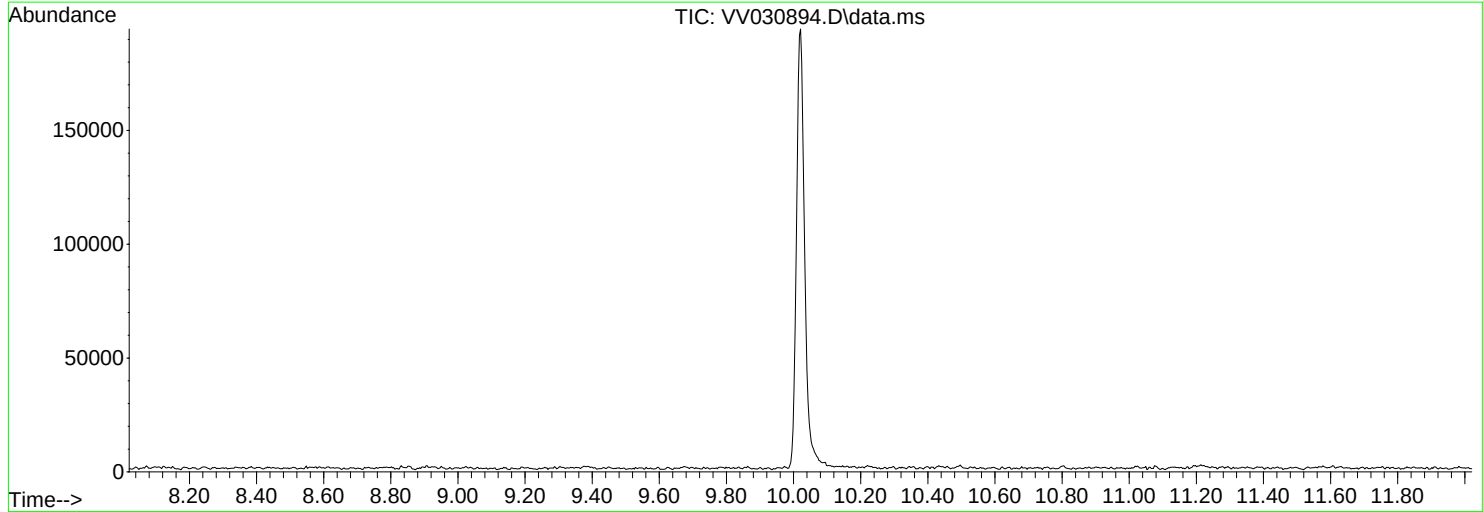

AutoFind: Scans 2792, 2793, 2794; Background Corrected with Scan 2781

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	6488	PASS
75	95	30	80	52.6	17211	PASS
95	95	100	100	100.0	32699	PASS
96	95	5	9	6.5	2119	PASS
173	174	0.00	2	1.9	653	PASS
174	95	50	120	103.1	33712	PASS
175	174	5	9	8.7	2918	PASS
176	174	95	105	101.6	34235	PASS
177	176	5	10	6.4	2177	PASS

m/z	Abundance
35.80	149.0
38.30	135.0
39.40	140.0
39.80	150.0
40.10	153.0
41.90	123.0
43.90	275.0
50.80	132.0
59.80	111.0
91.00	154.0

Instrument :
MSVOA_V
ClientSampleId :
BFB374

m/z	Abundance
36.10	447.0
37.00	1942.0
38.00	1874.0
39.10	736.0
40.00	231.0
41.20	116.0
42.00	101.0
42.90	155.0
43.90	438.0
44.90	480.0
45.80	170.0
47.00	522.0
48.10	268.0
49.00	1501.0
50.00	6800.0
51.10	2069.0
51.90	195.0
53.10	159.0
55.10	139.0
56.00	585.0
57.00	1179.0
58.00	144.0
60.00	464.0
61.00	1819.0
62.00	2199.0
63.00	1900.0
63.90	279.0
65.10	393.0
67.00	164.0
68.00	3467.0
69.00	3761.0
70.00	329.0
72.10	233.0
73.10	1837.0
74.10	6020.0
75.00	17448.0
76.00	1595.0
76.90	204.0
78.00	196.0
78.90	1794.0
80.00	521.0
80.90	1840.0
81.90	437.0
82.90	108.0
87.00	1108.0
88.00	1441.0
91.00	208.0
92.00	1405.0
93.00	1785.0
94.00	4369.0
95.00	33336.0
96.00	2302.0
103.90	296.0
104.70	102.0
105.90	232.0
115.90	192.0
117.00	387.0
117.80	254.0
118.90	292.0
128.00	186.0
129.00	100.0
130.00	227.0
134.90	103.0
136.90	221.0
141.10	429.0
141.80	139.0
142.90	646.0
145.00	188.0
154.90	141.0
157.00	102.0
158.80	171.0
171.90	440.0
173.00	635.0
174.00	33712.0
174.90	2925.0
176.00	34080.0
177.00	2222.0
178.00	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB374

m/z	Abundance
36.10	473.0
37.10	1850.0
38.10	2029.0
39.00	726.0
40.10	216.0
41.10	124.0
42.00	120.0
42.90	146.0
44.00	487.0
44.90	439.0
46.20	173.0
47.00	523.0
48.10	264.0
49.00	1612.0
50.00	6620.0
51.10	1939.0
51.90	196.0
53.10	126.0
53.70	109.0
55.00	133.0
56.00	659.0
57.00	1149.0
58.00	160.0
59.90	464.0
61.00	1884.0
62.00	2162.0
63.00	1852.0
63.90	277.0
65.10	387.0
67.00	180.0
68.00	3442.0
69.00	3809.0
70.00	372.0
72.00	268.0
73.10	1701.0
74.10	6327.0
75.10	17760.0
76.00	1533.0
77.00	259.0
78.00	211.0
78.90	1776.0
80.00	530.0
80.90	1822.0
81.90	418.0
87.00	1110.0
88.00	1351.0
90.90	225.0
92.00	1397.0
93.00	1785.0
94.00	4151.0
95.00	33648.0
96.10	2222.0
103.90	297.0
105.90	232.0
111.20	119.0
114.70	105.0
115.80	168.0
117.10	360.0
117.80	212.0
118.90	311.0
128.00	205.0
129.00	106.0
130.00	238.0
134.90	112.0
137.00	157.0
141.10	444.0
141.80	131.0
142.90	659.0
144.90	228.0
154.90	146.0
158.70	133.0
171.90	449.0
173.00	668.0
174.00	34624.0
174.90	3025.0
176.00	35432.0
176.90	2262.0
178.00	114.0

Instrument :
MSVOA_V
ClientSampleId :
BFB374

m/z	Abundance
36.10	455.0
37.00	1666.0
38.00	1890.0
39.00	665.0
40.10	213.0
41.10	159.0
41.90	118.0
42.90	113.0
44.00	467.0
44.90	353.0
46.20	182.0
47.10	448.0
48.00	228.0
49.00	1483.0
50.00	6045.0
51.00	1799.0
51.90	175.0
53.00	119.0
53.80	104.0
54.90	134.0
56.10	675.0
57.10	1040.0
58.00	149.0
60.00	411.0
61.00	1729.0
62.00	1888.0
63.00	1671.0
63.90	324.0
65.10	370.0
66.90	160.0
68.00	3304.0
69.00	3466.0
70.00	351.0
72.00	284.0
73.00	1532.0
74.10	6153.0
75.10	16424.0
76.00	1324.0
77.00	272.0
78.00	201.0
78.90	1570.0
80.00	459.0
80.90	1639.0
81.90	375.0
87.00	1104.0
88.00	1190.0
90.80	235.0
92.00	1264.0
93.00	1607.0
94.00	3807.0
95.00	31112.0
96.10	1832.0
103.90	277.0
105.90	217.0
114.80	113.0
115.70	181.0
117.10	257.0
117.80	206.0
118.90	318.0
127.90	178.0
130.10	209.0
134.90	121.0
137.20	134.0
141.00	380.0
141.80	111.0
142.90	605.0
144.80	259.0
148.20	104.0
154.90	118.0
171.90	366.0
173.10	657.0
174.00	32800.0
174.90	2803.0
176.00	33192.0
176.90	2047.0
178.00	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB374