
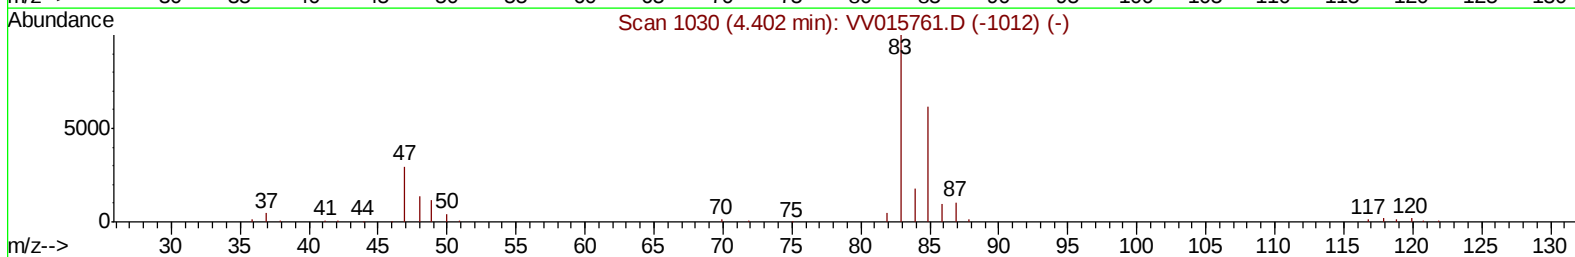
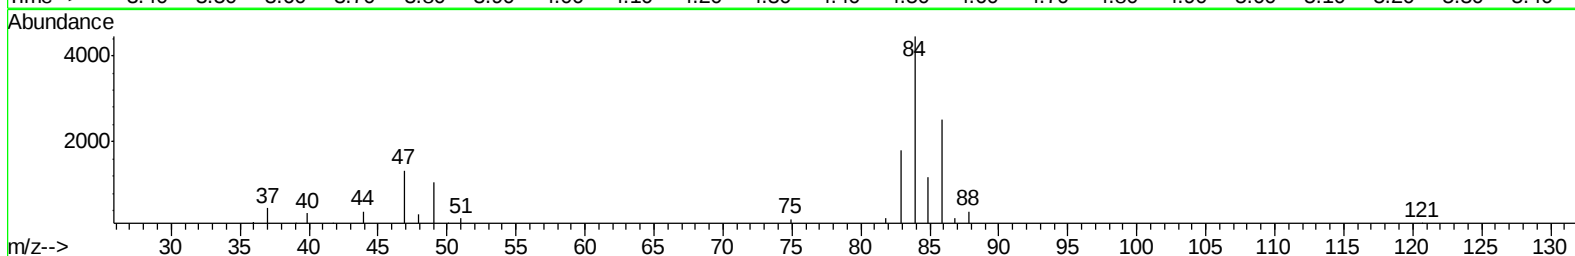


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV042820\
Data File : VV015764.D
Acq On : 28 Apr 2020 22:42
Operator : SY/MD
Sample : L2421-19
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 26 Sample Multiplier: 1

Quant Time: Apr 29 03:48:25 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Apr 29 03:36:29 2020
Response via : Initial Calibration

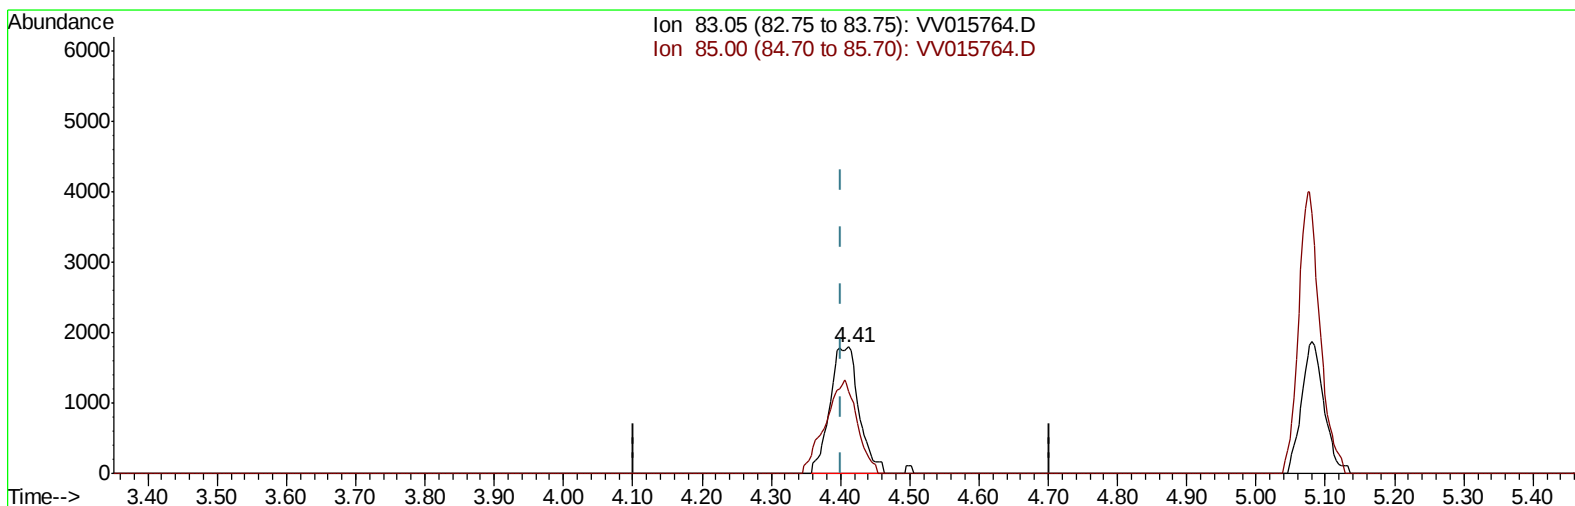

TIC: VV015764.D

(25) Chloroform (T)

4.412min (+0.010) 0.32ug/L m

response 5215

Ion	Exp%	Act%
83.05	100	100
85.00	65.80	65.18
0.00	0.00	0.00
0.00	0.00	0.00