

Quantitation Report (QT/LSC Reviewed)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV042820\
 Data File : VV015770.D
 Acq On : 29 Apr 2020 01:03
 Operator : SY/MD
 Sample : L2419-01
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AE6

Manual Integrations
 APPROVED

apatel
 5/1/2020 12:32:06 PM

Quant Time: Apr 29 05:41:53 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Apr 29 03:36:29 2020
 Response via : Initial Calibration

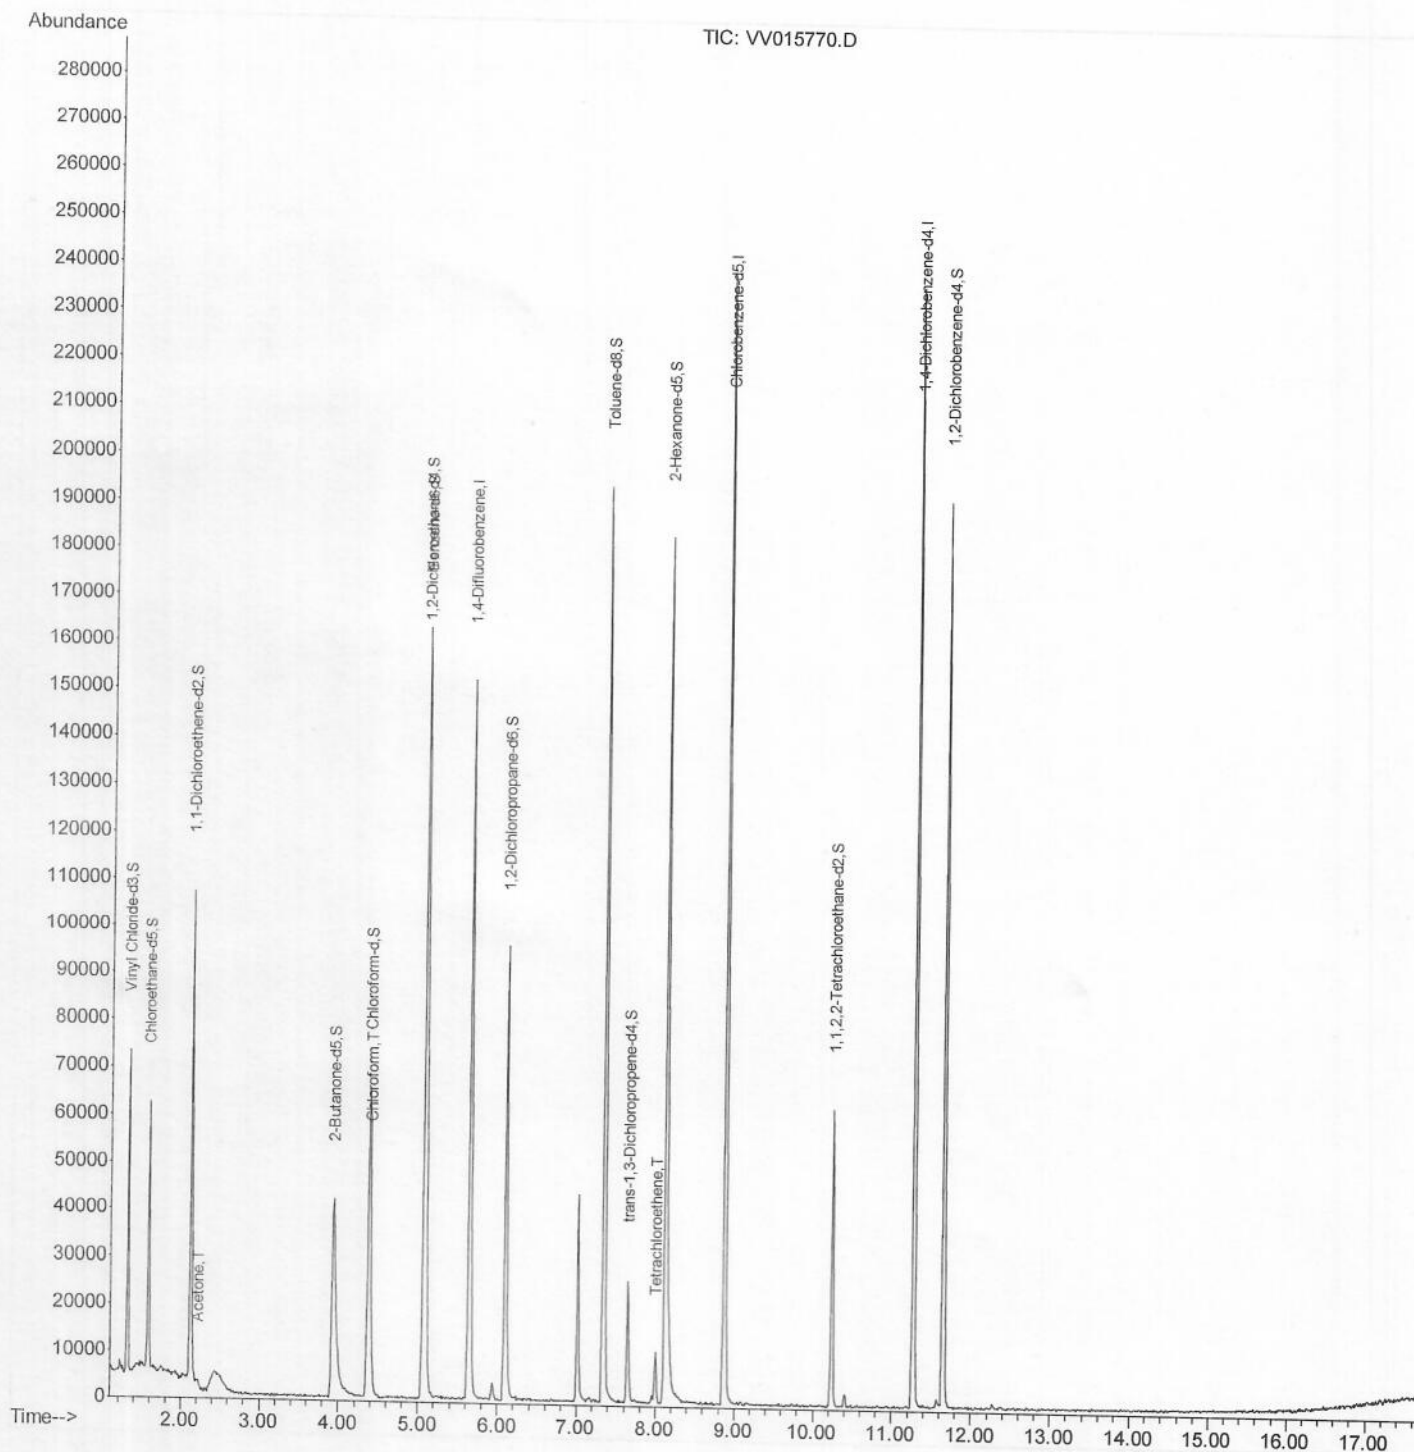

Quantitation Report (Qedit)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV042820\
 Data File : VV015770.D
 Acq On : 29 Apr 2020 01:03
 Operator : SY/MD
 Sample : L2419-01
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampled :
 C0AE6

Manual Integrations
 APPROVED

apatel
 5/1/2020 12:32:06 PM

Quant Time: Apr 29 03:49:46 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Apr 29 03:36:29 2020
 Response via : Initial Calibration

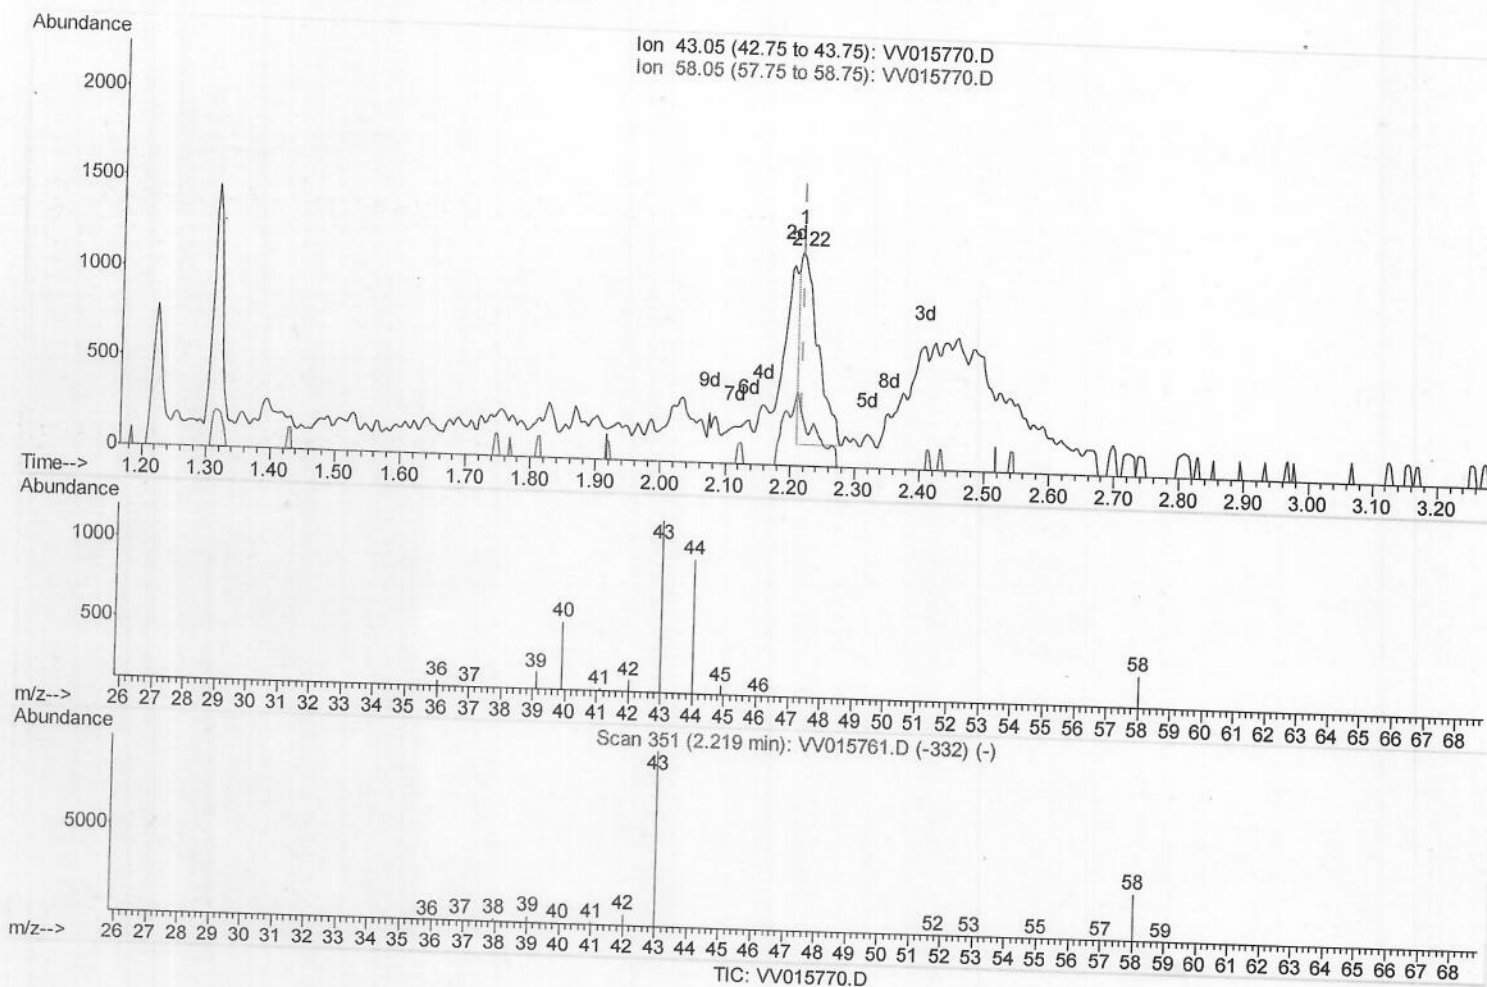

(13) Acetone (T)

2.216min (-0.003) 1.46ug/L

response 2041

Ion	Exp%	Act%
43.05	100	100
58.05	28.80	24.25
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV042820\
 Data File : VV015770.D
 Acq On : 29 Apr 2020 01:03
 Operator : SY/MD
 Sample : L2419-01
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AE6

Manual Integrations
 APPROVED

apatel
 5/1/2020 12:32:06 PM

Quant Time: Apr 29 03:49:46 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Apr 29 03:36:29 2020
 Response via : Initial Calibration

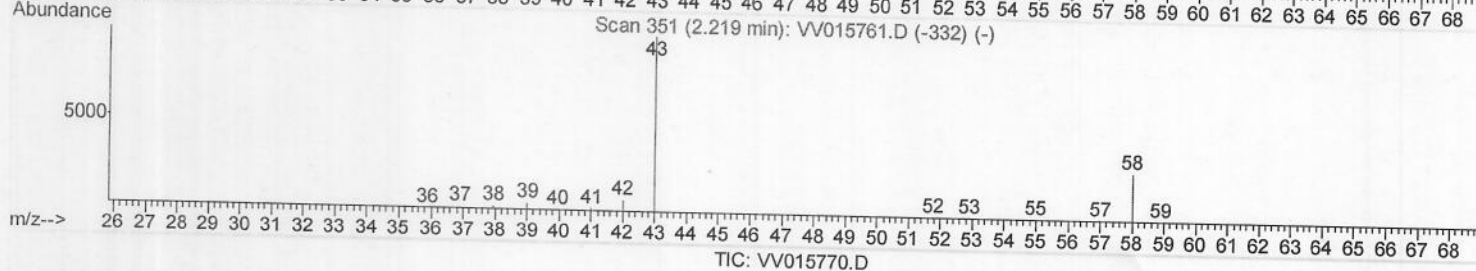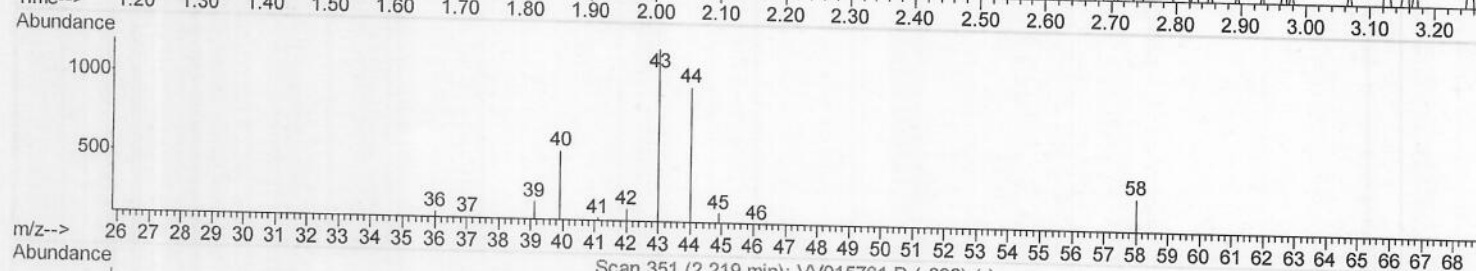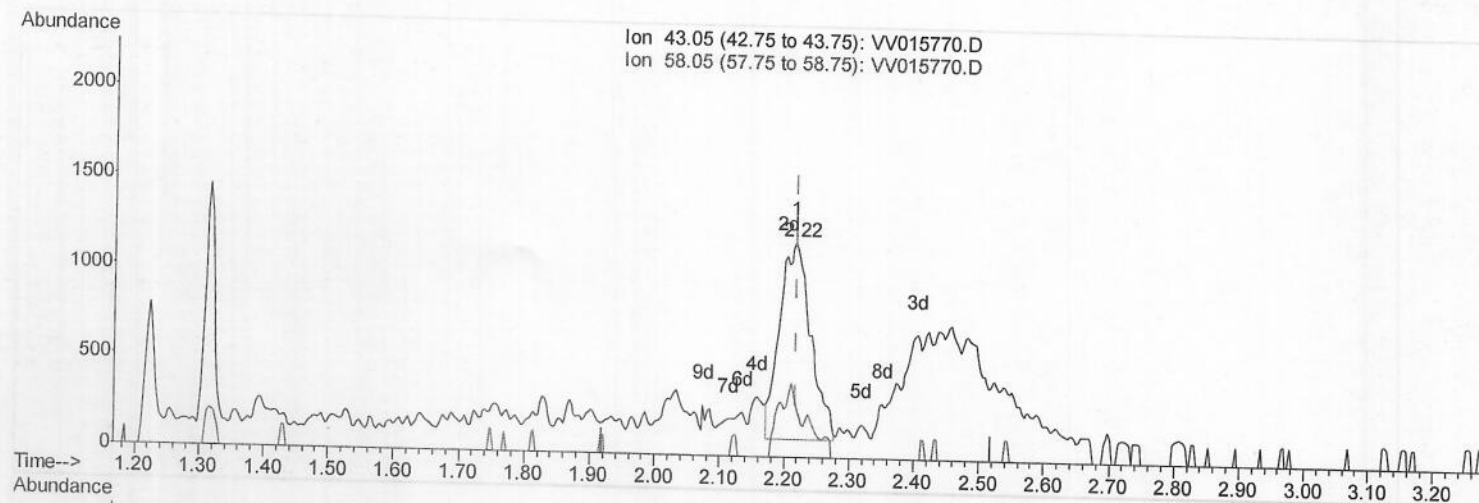

(13) Acetone (T)

2.216min (-0.003) 2.59ug/L m

response 3627

Ion	Exp%	Act%
43.05	100	100
58.05	28.80	13.65
0.00	0.00	0.00
0.00	0.00	0.00

MD
 05/5/2020

Quantitation Report (QT/LSC Reviewed)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV042820\
 Data File : VV015770.D
 Acq On : 29 Apr 2020 01:03
 Operator : SY/MD
 Sample : L2419-01
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 Client Sample ID :
 C0AE6

Manual Integrations
 APPROVED

apatel
 5/1/2020 12:32:06 PM

Quant Time: Apr 29 05:41:53 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Apr 29 03:36:29 2020
 Response via : Initial Calibration

Internal Standards		R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene		5.64	114	120340	5.00	ug/L	0.00
28) Chlorobenzene-d5		8.87	117	117083	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4		11.27	152	54428	5.00	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		1.32	65	39152	6.23	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	124.60%	
7) Chloroethane-d5		1.58	69	33292	5.49	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	109.80%	
11) 1,1-Dichloroethene-d2		2.12	63	56118	4.08	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	81.60%	
20) 2-Butanone-d5		3.93	46	91501	45.31	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	90.62%	
24) Chloroform-d		4.38	84	63665	4.34	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.80%	
26) 1,2-Dichloroethane-d4		5.06	65	41432	5.05	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.00%	
32) Benzene-d6		5.08	84	137331	4.91	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.20%	
36) 1,2-Dichloropropane-d6		6.09	67	41118	4.60	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	92.00%	
41) Toluene-d8		7.34	98	120736	4.55	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.00%	
43) trans-1,3-Dichloropropene-		7.64	79	13930	4.03	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.60%	
46) 2-Hexanone-d5		8.11	63	61754	36.67	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	73.34%	
57) 1,1,2,2-Tetrachloroethane-		10.24	84	27913	4.20	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	84.00%	
64) 1,2-Dichlorobenzene-d4		11.65	152	43952	4.75	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.00%	
Target Compounds							
13) Acetone		2.22	43	3627m	2.587	ug/L	Ovalue
25) Chloroform		4.40	83	7400	0.453	ug/L	97
47) Tetrachloroethene		8.00	164	2430	0.365	ug/L	89

MD
 05/5/2020

(#) = qualifier out of range (m) = manual integration (+) = signals summed