

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV042820\
 Data File : VV015748.D
 Acq On : 28 Apr 2020 15:41
 Operator : SY/MD
 Sample : L2413-22
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Quant Time: Apr 29 01:25:27 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Apr 29 00:40:59 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	125157	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	123409	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	57818	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	40293	6.16	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	123.20%
7) Chloroethane-d5	1.57	69	34066	5.40	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	108.00%
11) 1,1-Dichloroethene-d2	2.12	63	58215	4.07	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	81.40%
20) 2-Butanone-d5	3.96	46	90328	43.01	ug/L	0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	86.02%
24) Chloroform-d	4.38	84	66714	4.38	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.60%
26) 1,2-Dichloroethane-d4	5.06	65	42236	4.95	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.00%
32) Benzene-d6	5.07	84	140785	4.78	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.60%
36) 1,2-Dichloropropane-d6	6.09	67	43637	4.64	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	92.80%
41) Toluene-d8	7.34	98	125834	4.50	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.00%
43) trans-1,3-Dichloropropene-	7.65	79	14948	4.11	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.20%
46) 2-Hexanone-d5	8.12	63	67536	38.05	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	76.10%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	28768	4.10	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	82.00%
64) 1,2-Dichlorobenzene-d4	11.65	152	45717	4.65	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	93.00%


Target Compounds					Ovalue
25) Chloroform	4.41	83	5951	0.350 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV042820\
Data File : VV015748.D
Acq On : 28 Apr 2020 15:41
Operator : SY/MD
Sample : L2413-22
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Time: Apr 29 01:25:27 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Apr 29 00:40:59 2020
Response via : Initial Calibration

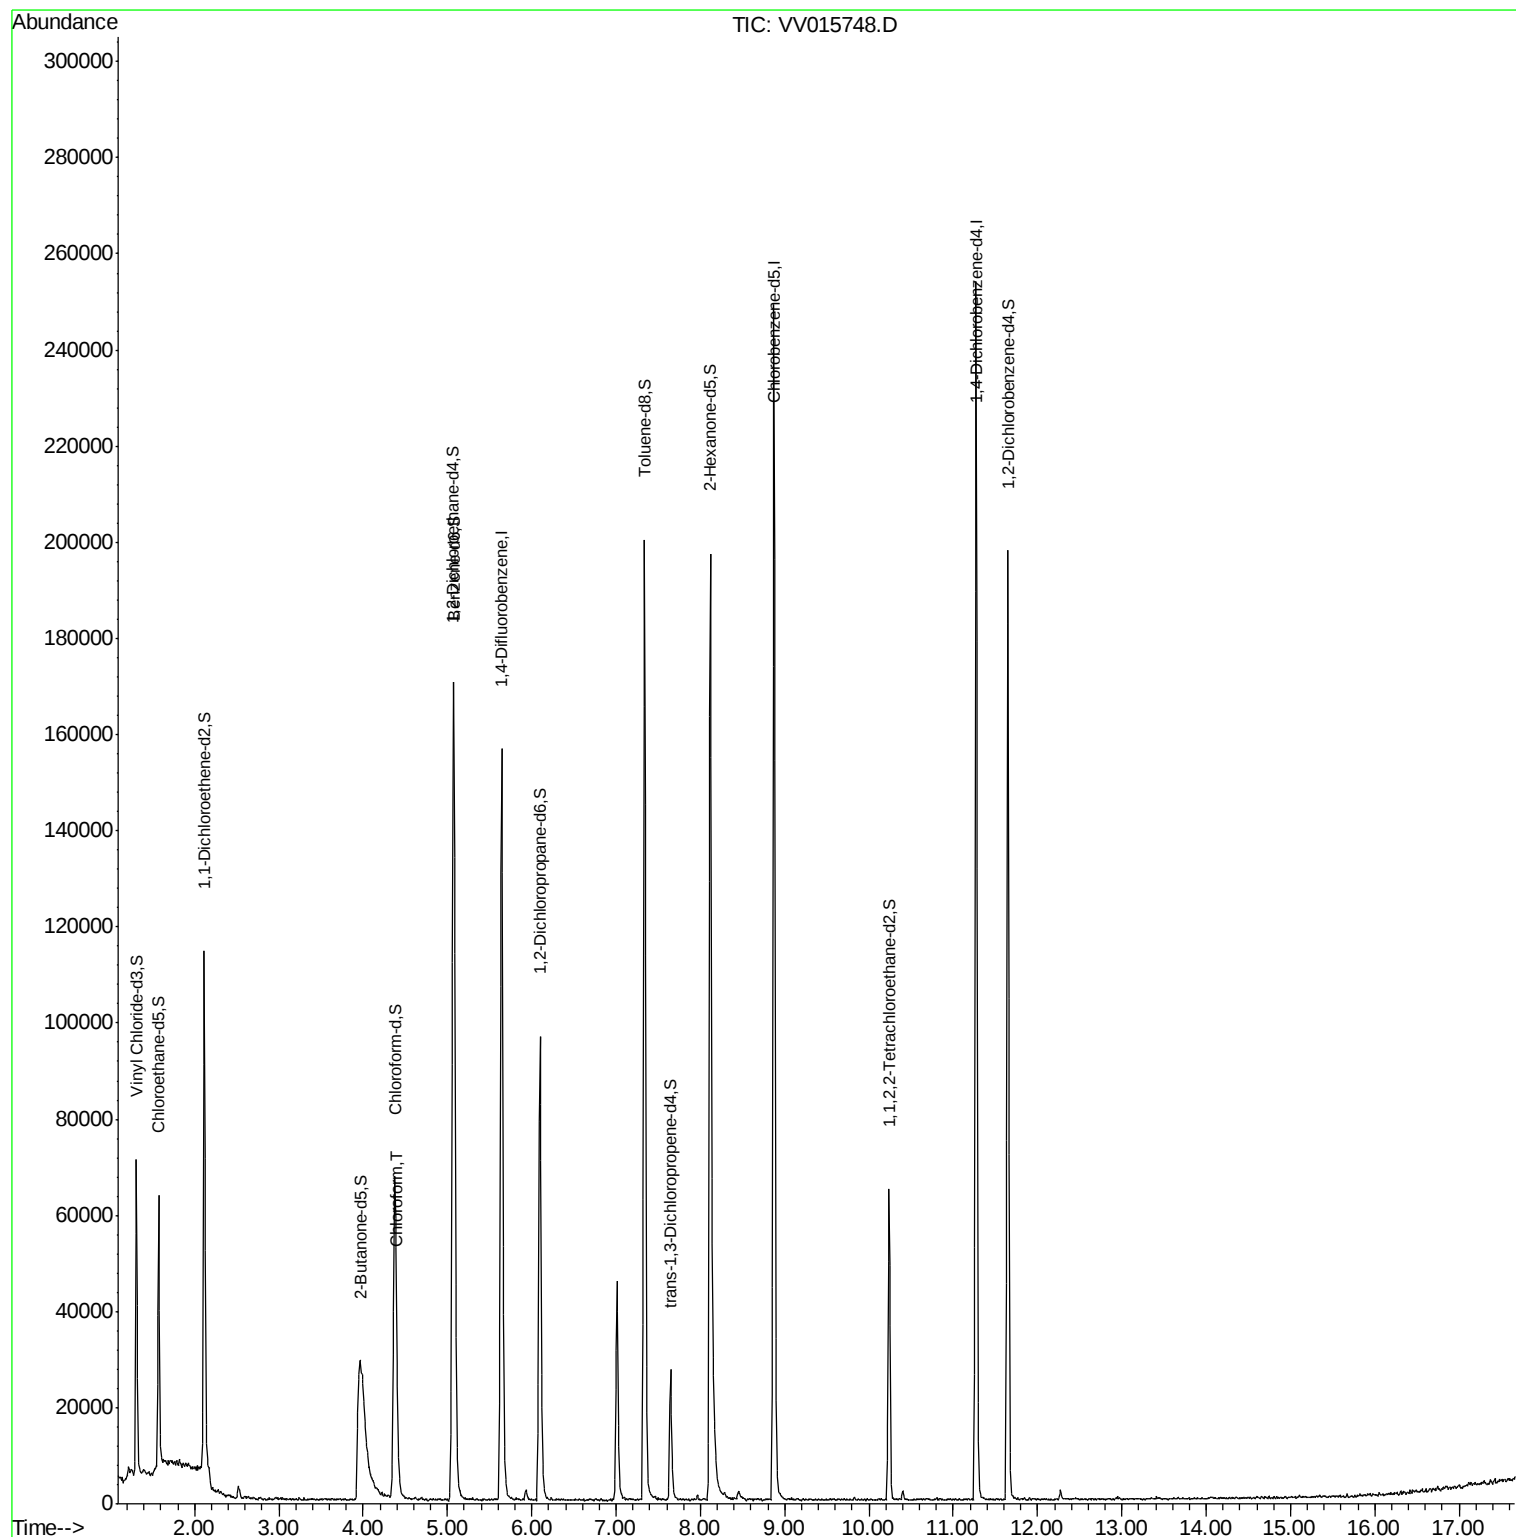

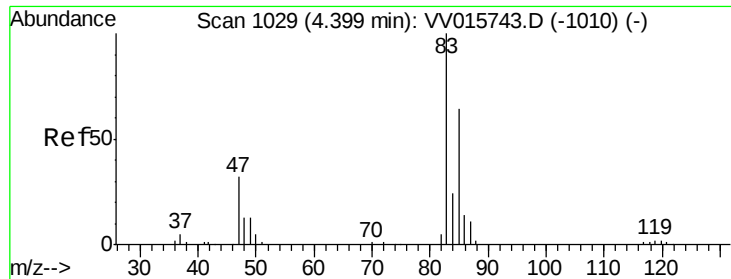

#25
 Chloroform
 Concen: 0.350 ug/L
 RT: 4.41 min Scan# 1031
 Delta R.T. 0.01 min
 Lab File: VV015748.D
 Acq: 28 Apr 2020 15:41

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Tot Ion: 83 Resp: 5951
 Ion Ratio Lower Upper
 83 100
 85 61.4 46.1 85.5

