

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV042820\
 Data File : VV015756.D
 Acq On : 28 Apr 2020 19:13
 Operator : SY/MD
 Sample : L2421-11
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFSB3

Quant Time: Apr 29 02:53:45 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Apr 29 00:40:59 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	124308	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	122567	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	57001	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	24278	3.74	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	74.80%
7) Chloroethane-d5	1.58	69	26955	4.31	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	86.20%
11) 1,1-Dichloroethene-d2	2.12	63	42097	2.96	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	59.20%#
20) 2-Butanone-d5	3.92	46	113015	54.18	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	108.36%
24) Chloroform-d	4.38	84	72070	4.76	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.20%
26) 1,2-Dichloroethane-d4	5.06	65	44348	5.23	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.60%
32) Benzene-d6	5.08	84	136172	4.65	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.00%
36) 1,2-Dichloropropane-d6	6.09	67	44867	4.80	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.00%
41) Toluene-d8	7.34	98	121291	4.36	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.20%
43) trans-1,3-Dichloropropene-	7.65	79	13636	3.77	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	75.40%
46) 2-Hexanone-d5	8.11	63	77676	44.06	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	88.12%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	32975	4.74	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.80%
64) 1,2-Dichlorobenzene-d4	11.65	152	48736	5.03	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.60%

Target Compounds


					Ovalue
13) Acetone	2.20	43	1765	1.219 ug/L	84
22) cis-1,2-Dichloroethene	3.95	96	4527	0.505 ug/L	85
34) Trichloroethene	5.94	95	12707	1.314 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV042820\
Data File : VV015756.D
Acq On : 28 Apr 2020 19:13
Operator : SY/MD
Sample : L2421-11
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFSB3

Quant Time: Apr 29 02:53:45 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Apr 29 00:40:59 2020
Response via : Initial Calibration

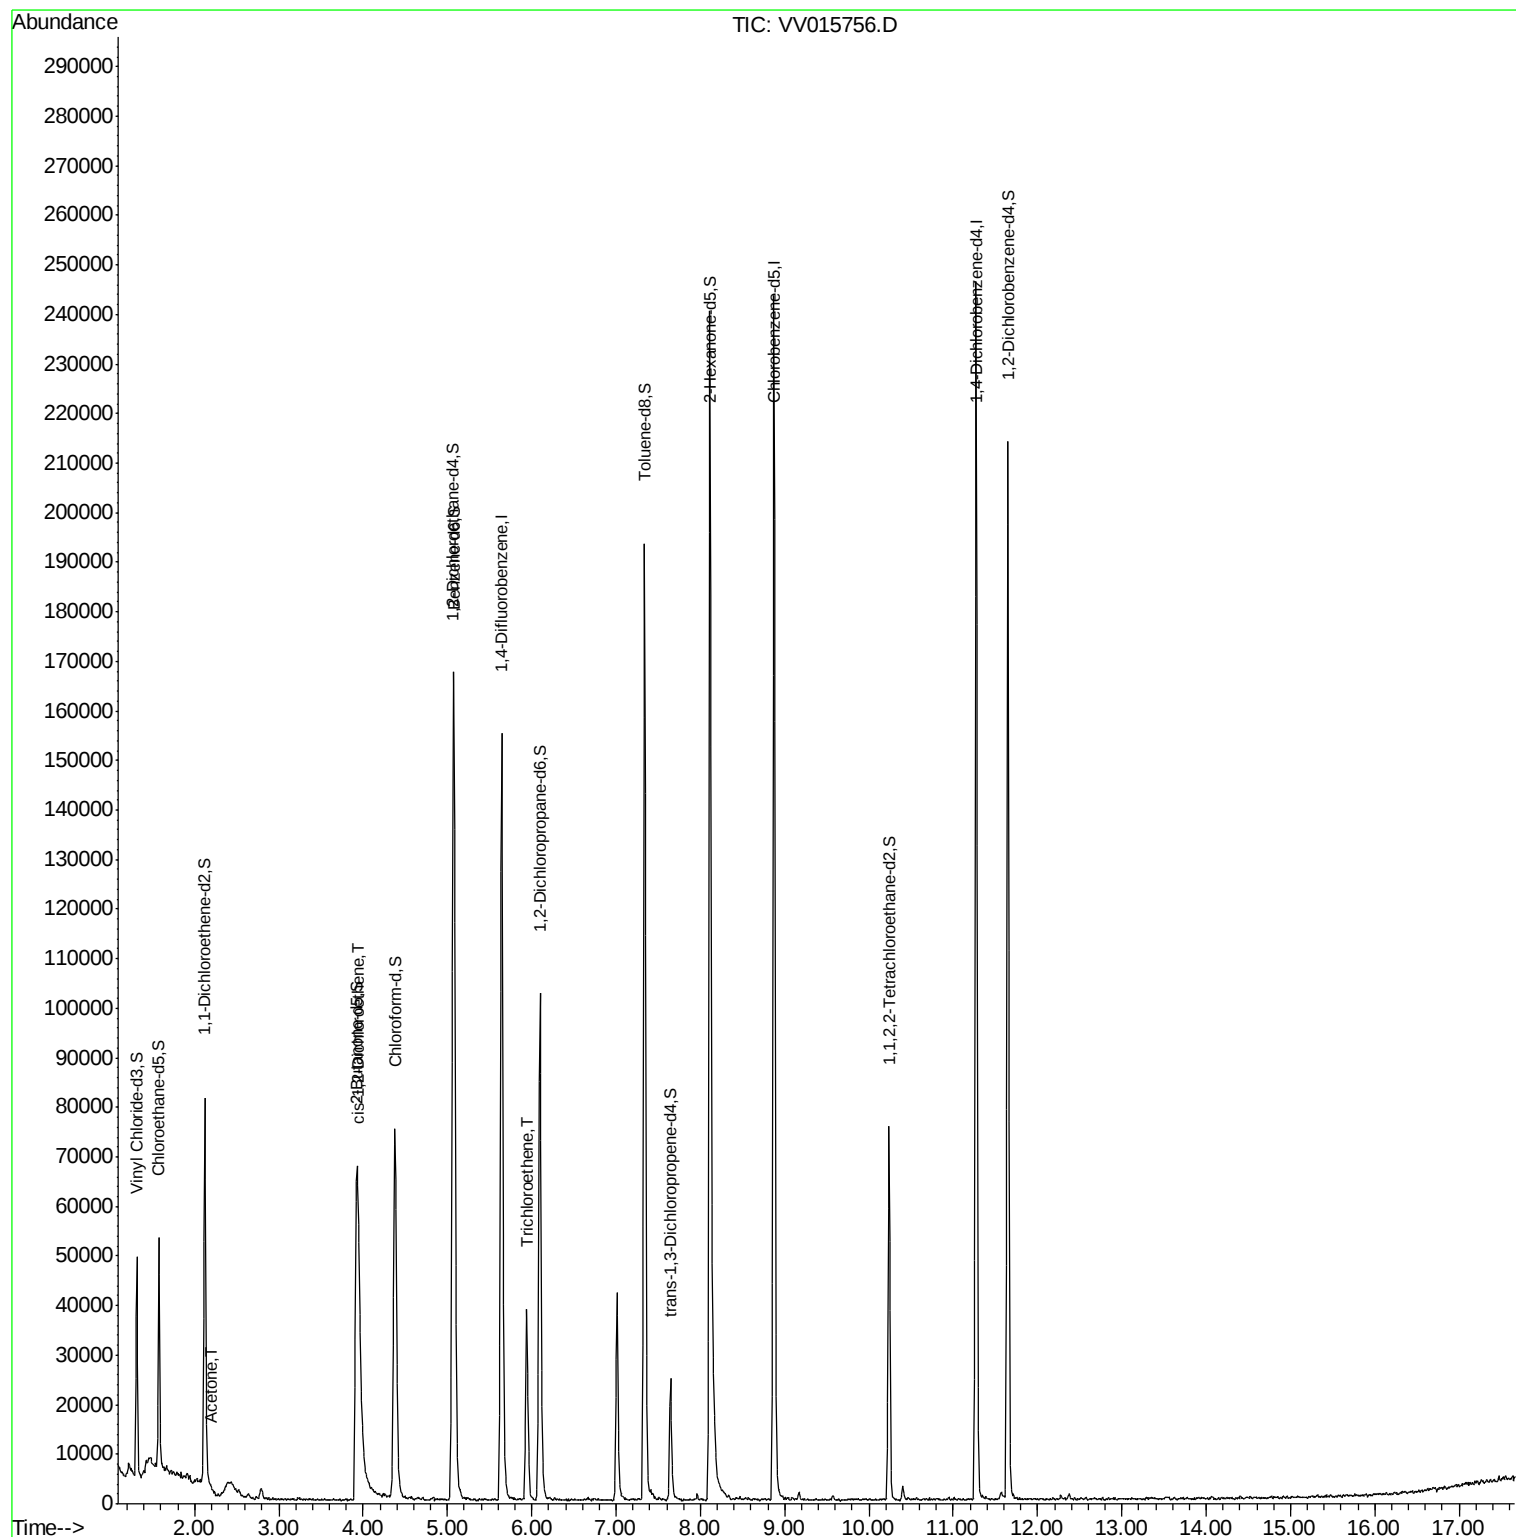

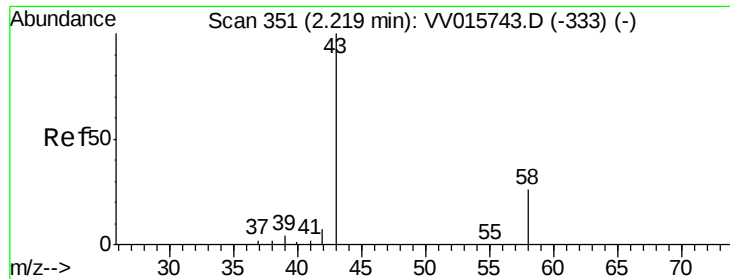

#13

Acetone

Concen: 1.219 ug/L

RT: 2.20 min Scan# 345

Delta R.T. -0.02 min

Lab File: VV015756.D

Acq: 28 Apr 2020 19:13

Instrument :

MSVOA_V

ClientSampled :


BFSB3

Tot Ion: 43 Resp: 1765

Ion Ratio Lower Upper




43 100

58 37.5 0.0 57.6

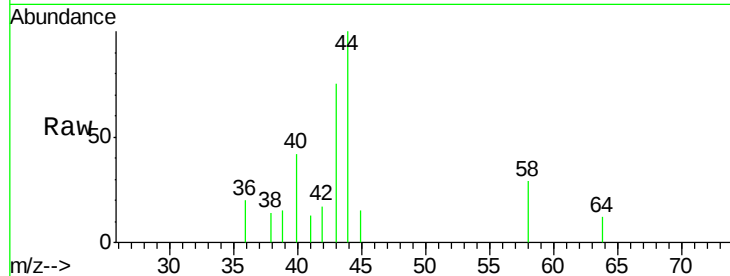

Abundance Ion 43.05 (42.75 to 43.75): VV0

Ion 58.05 (57.75 to 58.75): VV0

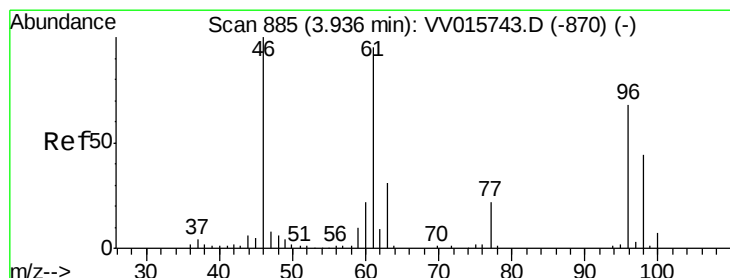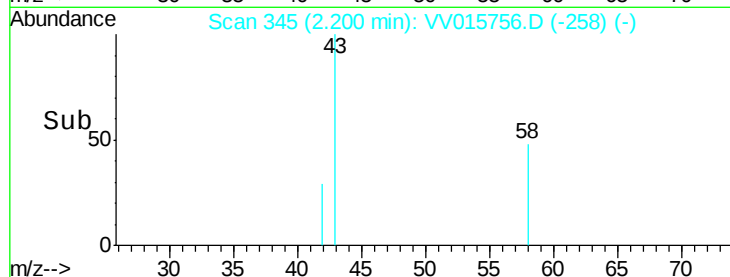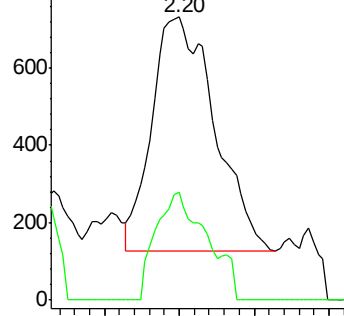

#22

cis-1,2-Dichloroethene

Concen: 0.505 ug/L

RT: 3.95 min Scan# 888

Delta R.T. 0.01 min

Lab File: VV015756.D

Acq: 28 Apr 2020 19:13


Tgt Ion: 96 Resp: 4527

Ion Ratio Lower Upper

96 100

61 155.7 96.4 179.0



68 0.0 0.0 0.0



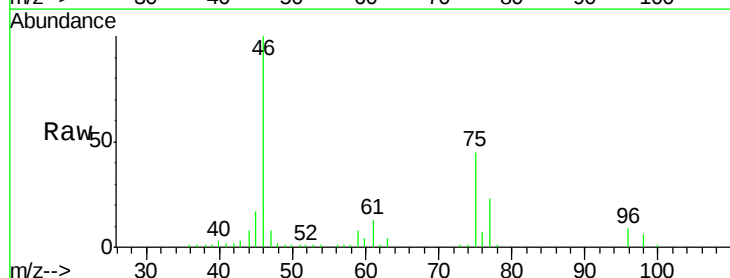


Abundance Ion 96.00 (95.70 to 96.70): VV0

Ion 61.05 (60.75 to 61.75): VV0

Ion 68.15 (67.85 to 68.85): VV0

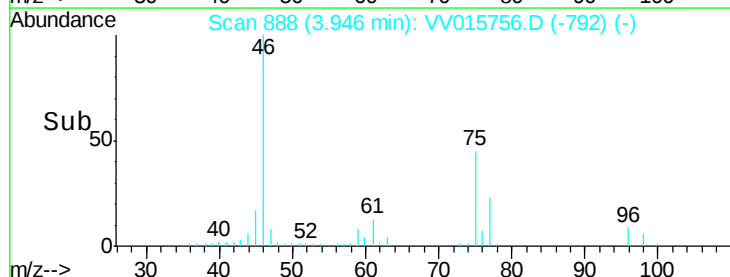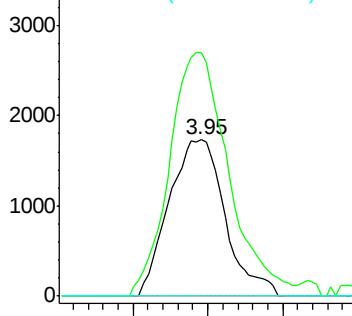

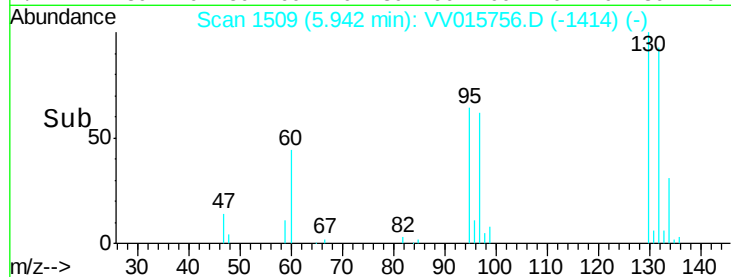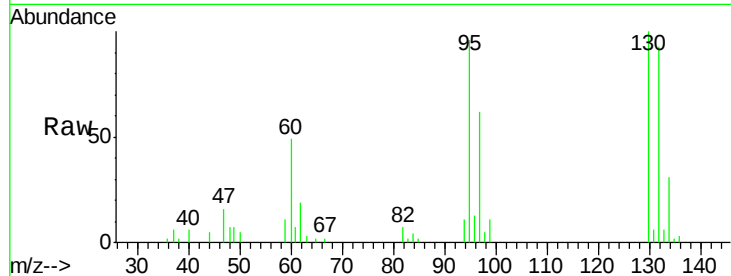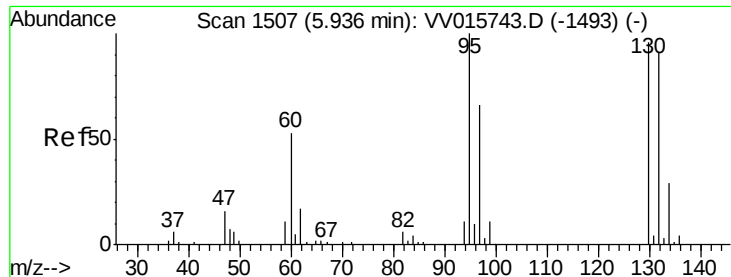

#34

Trichloroethene

Concen: 1.314 ug/L

RT: 5.94 min Scan# 1509

Delta R.T. 0.01 min

Lab File: VV015756.D

Acq: 28 Apr 2020 19:13

Instrument :

MSVOA_V

ClientSampleId :

BFSB3

Tot Ion: 95 Resp: 12707

Ion Ratio Lower Upper

95 100

97 64.5 44.7 82.9

132 96.7 65.2 121.0

130 104.4 65.0 120.6

Abundance Ion 95.00 (94.70 to 95.70): VV0

Ion 96.95 (96.65 to 97.65): VV0

Ion 131.95 (131.65 to 132.65): V

Ion 129.95 (129.65 to 130.65): V

