

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV042820\
 Data File : VV015762.D
 Acq On : 28 Apr 2020 21:55
 Operator : SY/MD
 Sample : VV0428WBL02
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK48

Quant Time: Apr 29 03:54:11 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Apr 29 03:36:29 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	121864	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	120611	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	56779	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	38739	6.08	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	121.60%
7) Chloroethane-d5	1.58	69	34541	5.63	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	112.60%
11) 1,1-Dichloroethene-d2	2.12	63	56230	4.03	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	80.60%
20) 2-Butanone-d5	3.93	46	91278	44.64	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	89.28%
24) Chloroform-d	4.38	84	65511	4.41	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.20%
26) 1,2-Dichloroethane-d4	5.06	65	40293	4.85	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.00%
32) Benzene-d6	5.08	84	135907	4.72	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.40%
36) 1,2-Dichloropropane-d6	6.10	67	43089	4.68	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.60%
41) Toluene-d8	7.34	98	121918	4.46	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.20%
43) trans-1,3-Dichloropropene-	7.65	79	13972	3.93	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	78.60%
46) 2-Hexanone-d5	8.11	63	62740	36.17	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	72.34%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	28002	4.09	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	81.80%
64) 1,2-Dichlorobenzene-d4	11.65	152	43514	4.51	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	90.20%


Target Compounds					Ovalue
25) Chloroform	4.41	83	7372	0.445 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV042820\
Data File : VV015762.D
Acq On : 28 Apr 2020 21:55
Operator : SY/MD
Sample : VV0428WBL02
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK48

Quant Time: Apr 29 03:54:11 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Apr 29 03:36:29 2020
Response via : Initial Calibration

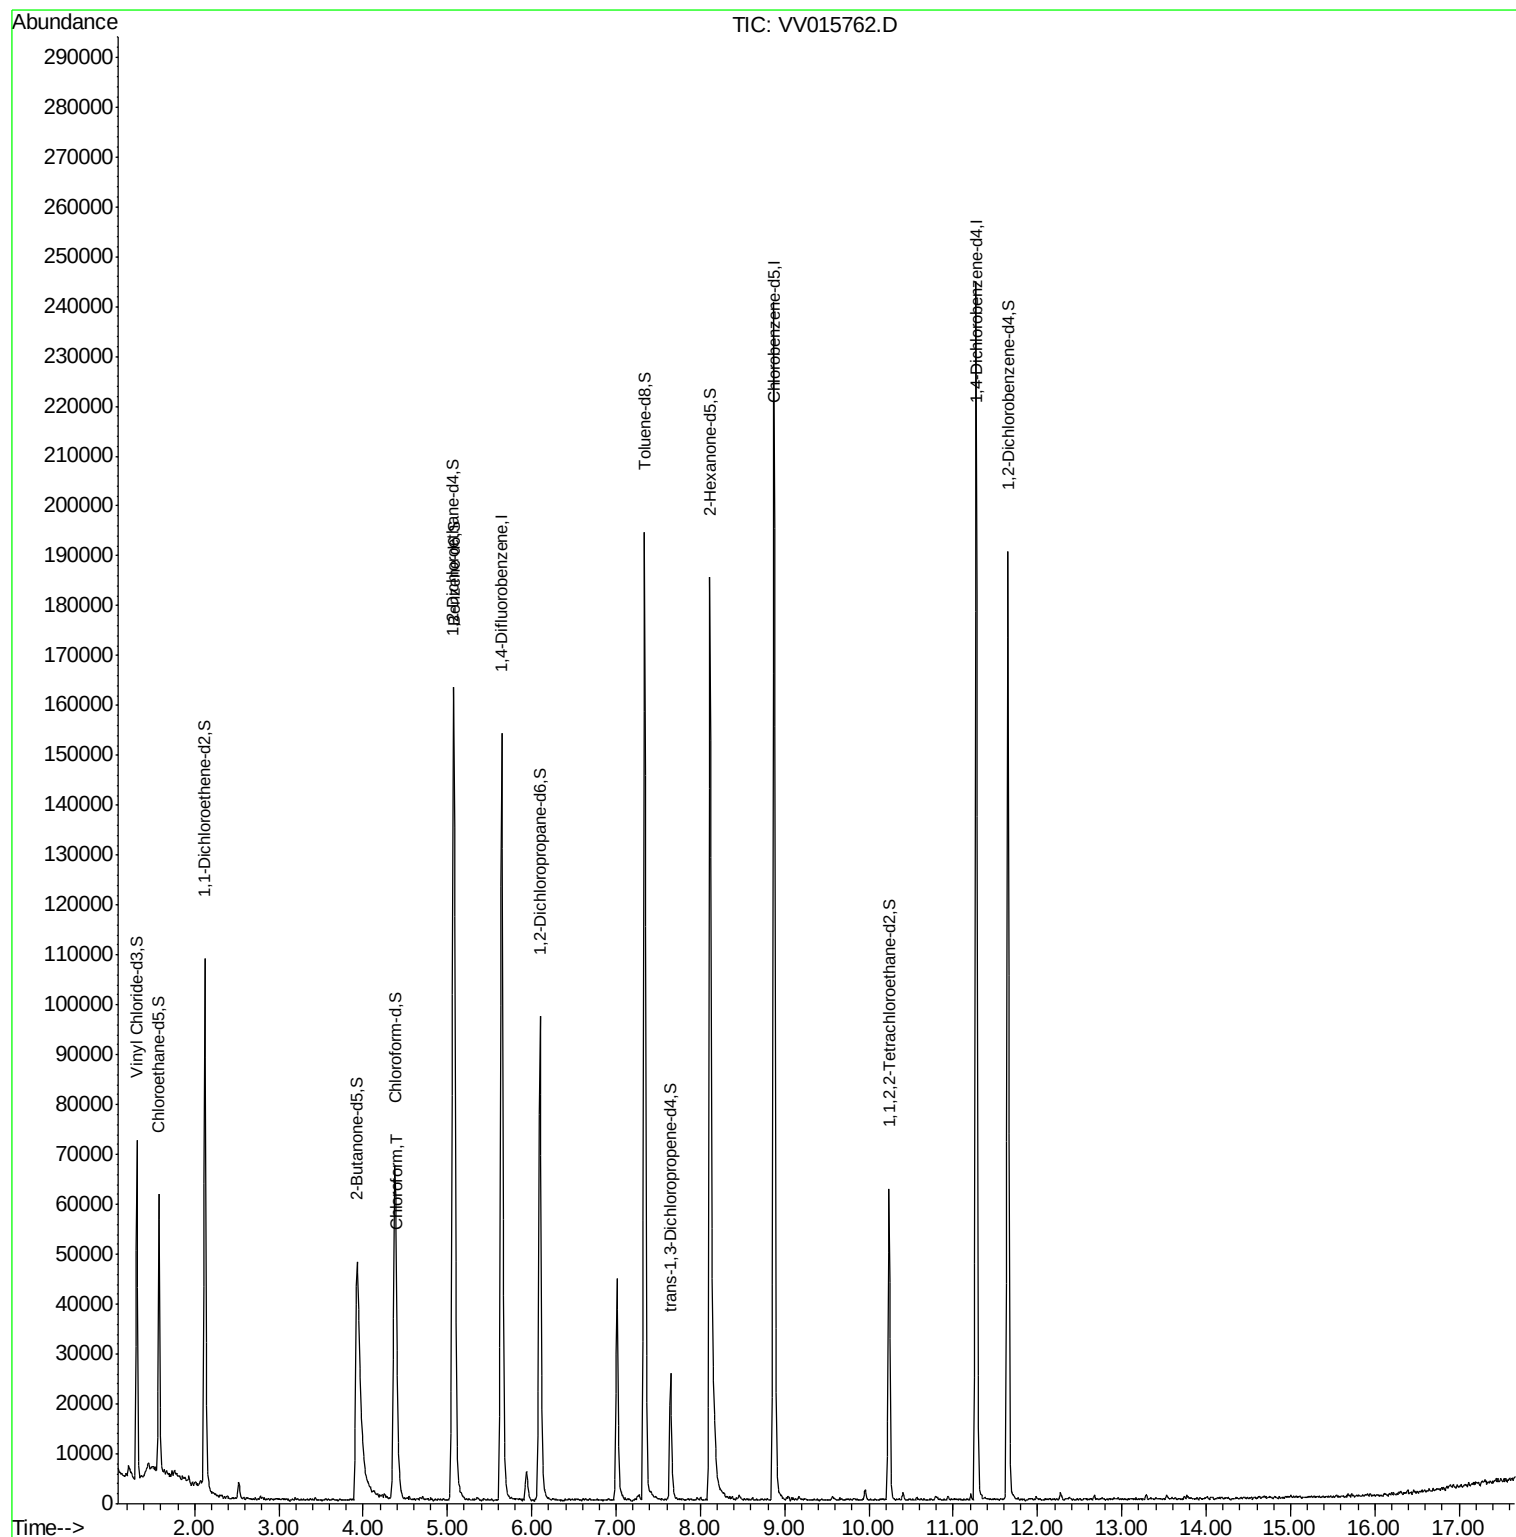

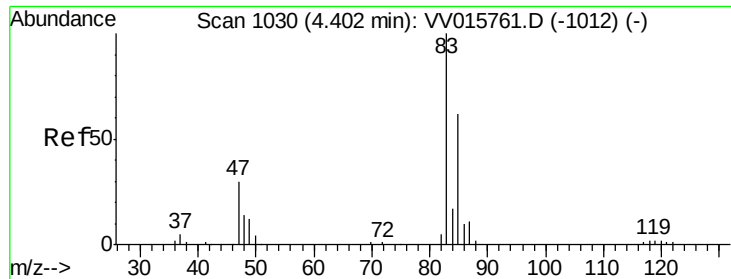

#25
 Chloroform
 Concen: 0.445 ug/L
 RT: 4.41 min Scan# 1031
 Delta R.T. 0.00 min
 Lab File: VV015762.D
 Acq: 28 Apr 2020 21:55

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK48

Tot Ion: 83 Resp: 7372
 Ion Ratio Lower Upper
 83 100
 85 63.7 46.1 85.5

