


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV042820\
 Data File : VV015742.D
 Acq On : 28 Apr 2020 09:56
 Operator : SY/MD
 Sample : BFB45
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB45

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Apr 29 03:36:29 2020

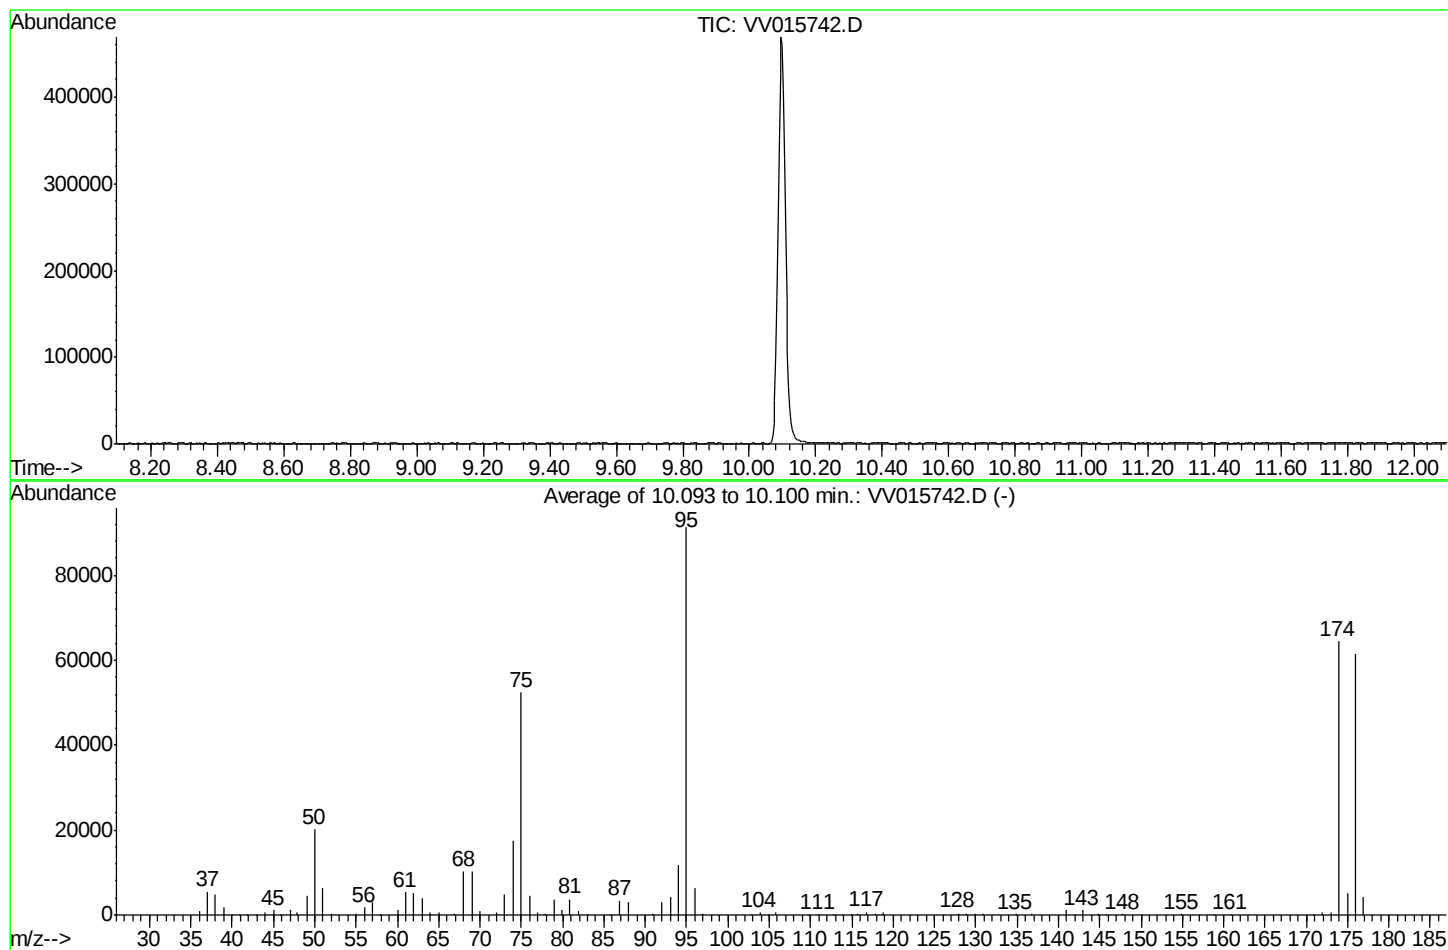

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2788

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.1	20194	PASS
75	95	30	80	57.3	52336	PASS
95	95	100	100	100.0	91306	PASS
96	95	5	9	7.0	6384	PASS
173	174	0.00	2	0.9	566	PASS
174	95	50	120	70.5	64408	PASS
175	174	5	9	7.8	5023	PASS
176	174	95	101	95.6	61565	PASS
177	176	5	9	6.7	4120	PASS

m/z	Abundance
36.00	1014.0
37.00	5294.0
38.00	4750.0
39.00	1901.0
40.00	414.0
43.00	108.0
44.00	1186.0
45.00	1021.0
45.90	111.0
47.00	1037.0
47.90	635.0
49.00	4232.0
50.00	19544.0
51.00	6040.0
51.90	269.0
55.00	321.0
56.00	1673.0
57.00	2957.0
57.90	114.0
60.00	1151.0
61.00	5197.0
62.00	4935.0
63.00	3718.0
63.90	541.0
65.00	559.0
67.00	372.0
68.00	9888.0
69.00	9920.0
70.00	732.0
72.00	618.0
73.00	4505.0
74.00	16704.0
75.00	49688.0
76.00	4225.0
77.00	639.0
77.90	412.0
78.90	3643.0
79.90	1121.0
80.90	3640.0
81.90	851.0
83.00	136.0
85.80	153.0
86.90	3111.0
87.90	2751.0
90.90	345.0
92.00	2871.0
93.00	3999.0
94.00	10918.0
95.00	86480.0
96.00	6256.0
97.00	204.0
103.80	550.0
104.80	121.0
105.80	522.0
109.60	120.0
111.00	151.0
112.80	122.0
114.80	127.0
115.80	347.0
116.80	735.0
117.80	335.0
118.80	602.0
127.90	343.0
128.90	162.0
129.90	300.0
130.90	197.0
134.90	246.0
136.70	188.0
141.00	1007.0
141.90	157.0
142.90	1169.0
144.80	244.0
145.80	123.0
147.80	190.0
150.00	144.0
154.80	232.0
157.10	137.0
160.90	126.0
170.80	118.0
171.90	646.0
173.00	830.0
173.90	58896.0
175.00	4763.0
175.90	56592.0
176.90	3899.0

Instrument :
MSVOA_V
ClientSampleId :
BFB45

m/z	Abundance
36.00	1100.0
37.00	5719.0
38.00	4964.0
39.00	1976.0
40.00	433.0
40.90	108.0
41.80	125.0
42.90	130.0
43.90	1143.0
45.00	1136.0
45.90	115.0
47.00	1170.0
47.90	695.0
49.00	4588.0
50.00	20984.0
51.00	6479.0
52.00	266.0
54.90	375.0
56.00	1797.0
57.00	3274.0
57.90	109.0
60.00	1166.0
61.00	5635.0
62.00	5332.0
63.00	3995.0
64.00	530.0
65.00	558.0
67.00	391.0
68.00	10615.0
69.00	10631.0
70.00	783.0
72.00	639.0
73.00	5127.0
74.00	18328.0
75.00	54456.0
76.00	4559.0
77.00	666.0
77.90	442.0
78.90	3813.0
79.90	1249.0
80.90	3811.0
81.90	947.0
82.90	135.0
85.90	133.0
86.90	3452.0
87.90	3126.0
90.90	366.0
92.00	3180.0
93.00	4413.0
94.00	12023.0
95.00	94504.0
96.00	6673.0
97.00	197.0
102.80	122.0
103.80	559.0
104.90	148.0
105.80	520.0
109.60	128.0
110.90	151.0
112.80	138.0
114.90	126.0
115.70	378.0
116.80	788.0
117.90	386.0
118.80	676.0
126.00	110.0
127.90	326.0
128.90	203.0
129.90	302.0
130.90	214.0
134.90	223.0
136.80	203.0
140.90	1141.0
142.00	142.0
142.90	1165.0
144.80	245.0
145.80	134.0
147.80	227.0
150.00	112.0
154.90	216.0
157.10	159.0
158.70	106.0
160.80	172.0
171.90	665.0
173.00	870.0
173.90	66624.0
175.00	5257.0
175.90	63648.0
176.90	4223.0

Instrument :
MSVOA_V
ClientSampleId :
BFB45

m/z	Abundance
36.00	1054.0
37.00	5680.0
38.00	4715.0
39.00	1893.0
40.00	470.0
40.90	133.0
41.80	118.0
42.90	156.0
43.90	1035.0
45.00	1105.0
45.90	122.0
47.00	1165.0
47.90	674.0
49.00	4362.0
50.00	20056.0
51.00	6122.0
52.00	274.0
54.90	378.0
56.00	1642.0
57.00	3193.0
58.00	116.0
60.00	1047.0
61.00	5312.0
62.00	5273.0
63.00	3810.0
64.00	474.0
65.00	589.0
66.90	373.0
68.00	10243.0
69.00	10141.0
70.00	818.0
72.00	599.0
73.00	5135.0
74.00	17888.0
75.00	52864.0
76.00	4415.0
77.00	629.0
77.90	457.0
78.90	3581.0
79.90	1257.0
80.90	3742.0
81.90	886.0
82.90	114.0
86.90	3450.0
87.90	3283.0
90.90	376.0
92.00	2998.0
93.00	4292.0
94.00	11989.0
95.00	92936.0
96.00	6223.0
97.00	190.0
102.80	132.0
103.90	483.0
104.90	168.0
105.90	447.0
110.80	162.0
112.80	146.0
114.90	151.0
115.80	383.0
116.80	735.0
117.90	424.0
118.80	647.0
126.00	125.0
127.90	315.0
128.80	235.0
129.90	277.0
130.80	178.0
134.80	200.0
136.80	212.0
140.90	1121.0
142.10	132.0
142.90	1109.0
144.80	220.0
145.80	125.0
147.80	235.0
155.00	202.0
156.90	157.0
158.80	106.0
160.80	173.0
171.90	723.0
173.90	67704.0
175.00	5049.0
175.90	64456.0
177.00	4238.0

Instrument :
MSVOA_V
ClientSampleId :
BFB45

Scan 2788 (10.055 min): VV015742.D
BFB45

m/z	Abundance
39.90	348.0
44.00	384.0

Instrument :
MSVOA_V
ClientSampleId :
BFB45