

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042821\
 Data File : VV021199.D
 Acq On : 28 Apr 2021 14:17
 Operator : SY/MD
 Sample : M2165-11DL 10000X
 Misc : 6.72g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB3F2DL

Quant Time: Apr 29 04:14:13 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 29 04:12:32 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	803398	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	795846	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.255	152	387627	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	241010	36.51	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	73.02%		
7) Chloroethane-d5	1.571	69	199214	41.02	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	82.04%		
11) 1,1-Dichloroethene-d2	2.111	63	338495	27.80	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	55.60%#		
21) 2-Butanone-d5	3.899	46	289898	89.93	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	89.93%		
24) Chloroform-d	4.352	84	502967	42.74	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	85.48%		
26) 1,2-Dichloroethane-d4	5.037	65	310686	41.53	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	83.06%		
32) Benzene-d6	5.056	84	952549	44.94	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	89.88%		
36) 1,2-Dichloropropane-d6	6.075	67	297067	46.96	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	93.92%		
41) Toluene-d8	7.320	98	894650	43.61	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	87.22%		
43) trans-1,3-Dichloroprop...	7.625	79	145530	42.09	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	84.18%		
47) 2-Hexanone-d5	8.095	63	221420	88.24	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	88.24%		
56) 1,1,2,2-Tetrachloroeth...	10.223	84	418114	43.82	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	87.64%		
66) 1,2-Dichlorobenzene-d4	11.631	152	397089	51.86	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	103.72%		
Target Compounds						Qvalue
46) Tetrachloroethene	7.979	164	420881	76.64	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042821\
Data File : VV021199.D
Acq On : 28 Apr 2021 14:17
Operator : SY/MD
Sample : M2165-11DL 10000X
Misc : 6.72g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB3F2DL

Quant Time: Apr 29 04:14:13 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 29 04:12:32 2021
Response via : Initial Calibration

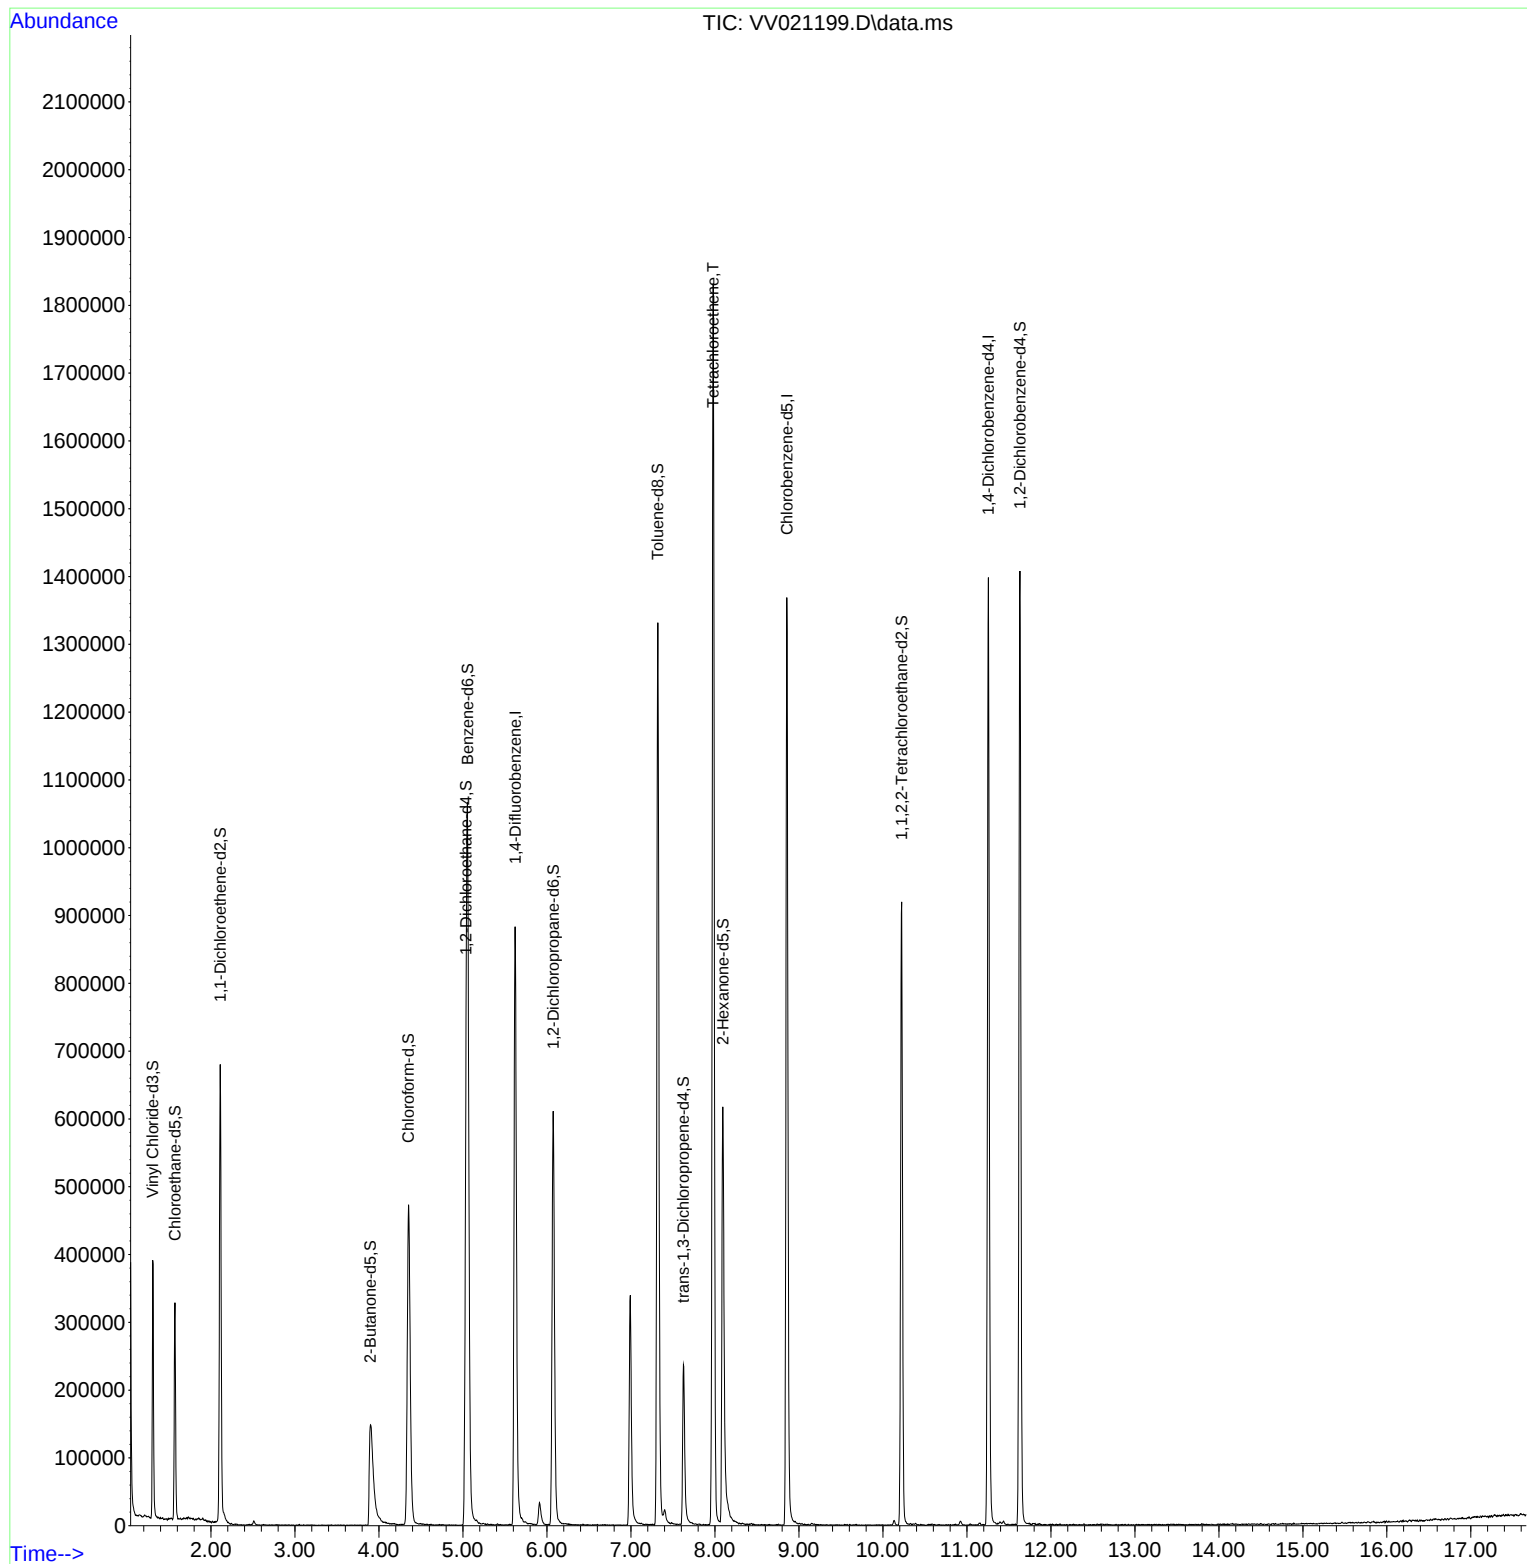

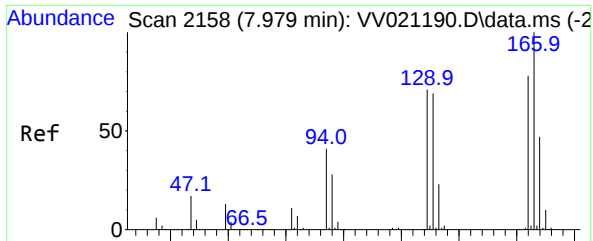

#46
Tetrachloroethene
Concen: 76.64 ug/L
RT: 7.979 min Scan# 2158
Delta R.T. -0.000 min
Lab File: VV021199.D
Acq: 28 Apr 2021 14:17

Instrument :
MSVOA_V
ClientSampleId :
GB3F2DL

Tgt Ion:164 Resp: 420881

Ion	Ratio	Lower	Upper
164	100		
129	91.2	63.8	118.4
131	85.7	59.3	110.1
166	125.0	87.7	162.9

