

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042821\
 Data File : VW021201.D
 Acq On : 28 Apr 2021 15:04
 Operator : SY/MD
 Sample : M2165-05DL 200X
 Misc : 5.44g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB3E6DL

Quant Time: Apr 29 04:14:25 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 29 04:12:32 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	797152	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	807207	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.255	152	404098	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	241929	36.93	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	73.86%		
7) Chloroethane-d5	1.571	69	199992	41.50	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	83.00%		
11) 1,1-Dichloroethene-d2	2.111	63	338029	27.98	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	55.96%#		
21) 2-Butanone-d5	3.902	46	304957	95.34	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	95.34%		
24) Chloroform-d	4.355	84	496328	42.50	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	85.00%		
26) 1,2-Dichloroethane-d4	5.037	65	308789	41.60	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	83.20%		
32) Benzene-d6	5.053	84	944183	43.92	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	87.84%		
36) 1,2-Dichloropropane-d6	6.076	67	298661	46.54	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	93.08%		
41) Toluene-d8	7.320	98	888647	42.71	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	85.42%		
43) trans-1,3-Dichloroprop...	7.625	79	143014	40.78	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	81.56%		
47) 2-Hexanone-d5	8.095	63	231792	91.07	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	91.07%		
56) 1,1,2,2-Tetrachloroeth...	10.220	84	423557	43.76	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	87.52%		
66) 1,2-Dichlorobenzene-d4	11.632	152	395979	49.61	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	99.22%		
Target Compounds						
					Qvalue	
46) Tetrachloroethene	7.979	164	553399	99.35	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042821\
Data File : VV021201.D
Acq On : 28 Apr 2021 15:04
Operator : SY/MD
Sample : M2165-05DL 200X
Misc : 5.44g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB3E6DL

Quant Time: Apr 29 04:14:25 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 29 04:12:32 2021
Response via : Initial Calibration

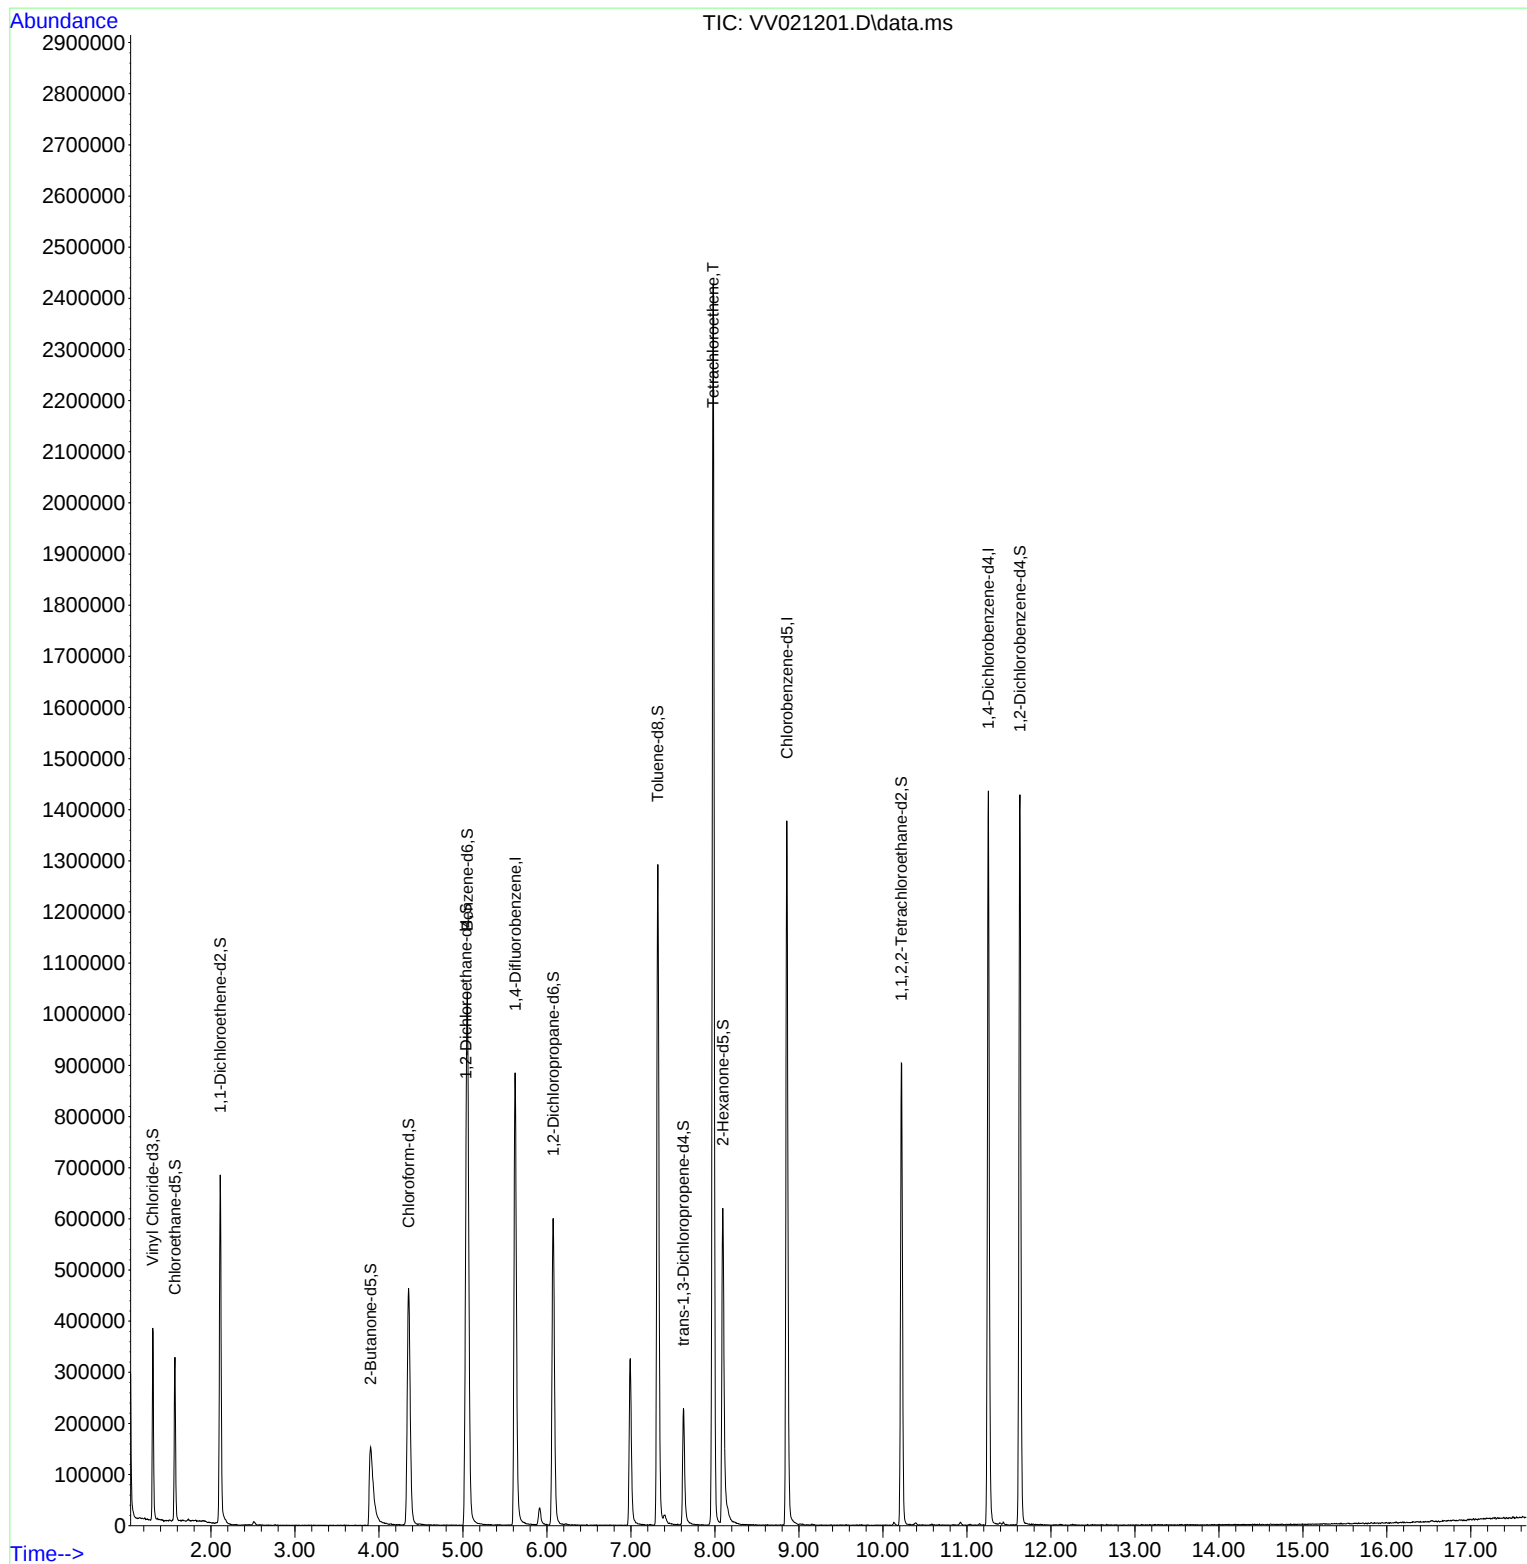

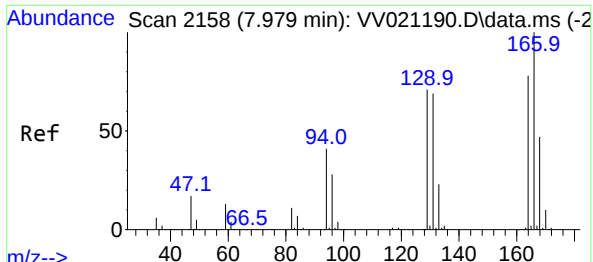

#46
Tetrachloroethene
Concen: 99.35 ug/L
RT: 7.979 min Scan# 2158
Delta R.T. 0.000 min
Lab File: VV021201.D
Acq: 28 Apr 2021 15:04

Instrument :
MSVOA_V
ClientSampleId :
GB3E6DL

Tgt Ion:164 Resp: 553399

Ion	Ratio	Lower	Upper
164	100		
129	91.0	63.8	118.4
131	88.0	59.3	110.1
166	129.6	87.7	162.9

