

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042821\
 Data File : VV021203.D
 Acq On : 28 Apr 2021 15:51
 Operator : SY/MD
 Sample : M2165-12DL 10000X
 Misc : 6.07g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB3F3DL

Quant Time: Apr 29 04:14:39 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 29 04:12:32 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	773555	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	781946	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.255	152	379236	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	252449	39.72	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	79.44%
7) Chloroethane-d5	1.571	69	210020	44.91	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	89.82%
11) 1,1-Dichloroethene-d2	2.108	63	358358	30.57	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	61.14%
21) 2-Butanone-d5	3.899	46	294272	94.81	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	94.81%
24) Chloroform-d	4.352	84	510612	45.06	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.12%
26) 1,2-Dichloroethane-d4	5.037	65	318753	44.25	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.50%
32) Benzene-d6	5.053	84	981209	47.12	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.24%
36) 1,2-Dichloropropane-d6	6.075	67	305749	49.19	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	98.38%
41) Toluene-d8	7.320	98	929587	46.12	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.24%
43) trans-1,3-Dichloroprop...	7.625	79	148295	43.65	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	87.30%
47) 2-Hexanone-d5	8.095	63	224338	90.99	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	90.99%
56) 1,1,2,2-Tetrachloroeth...	10.220	84	423366	45.15	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	90.30%
66) 1,2-Dichlorobenzene-d4	11.631	152	383027	51.13	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	102.26%
Target Compounds						
46) Tetrachloroethene	7.979	164	347970	64.49	ug/L	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042821\
Data File : VV021203.D
Acq On : 28 Apr 2021 15:51
Operator : SY/MD
Sample : M2165-12DL 10000X
Misc : 6.07g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB3F3DL


Quant Time: Apr 29 04:14:39 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 29 04:12:32 2021
Response via : Initial Calibration

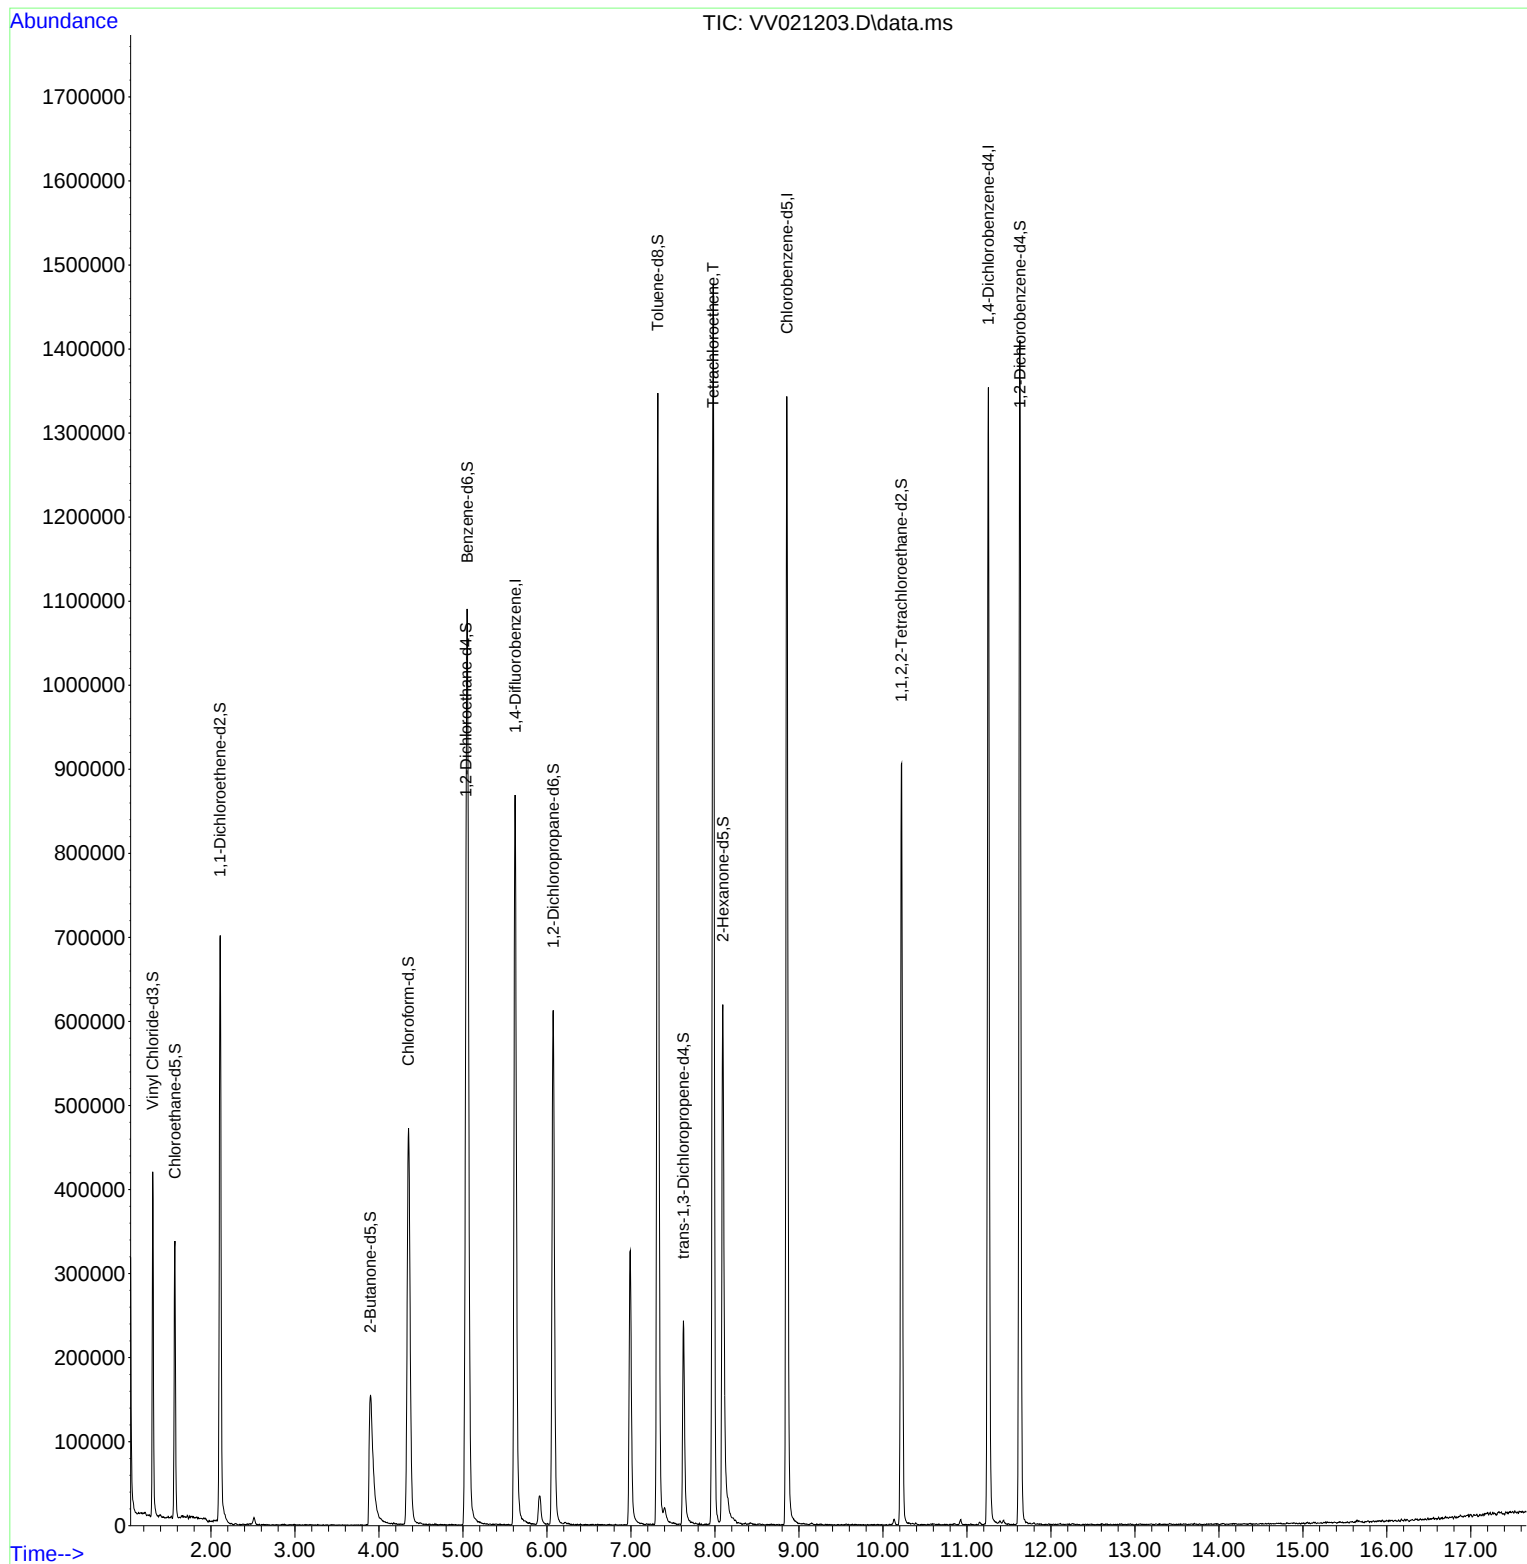

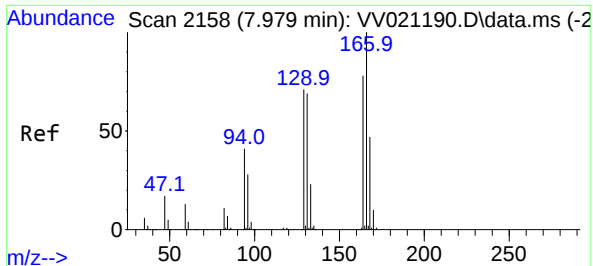

#46
Tetrachloroethene
Concen: 64.49 ug/L
RT: 7.979 min Scan# 2158
Delta R.T. -0.000 min
Lab File: VV021203.D
Acq: 28 Apr 2021 15:51

Instrument :
MSVOA_V
ClientSampleId :
GB3F3DL

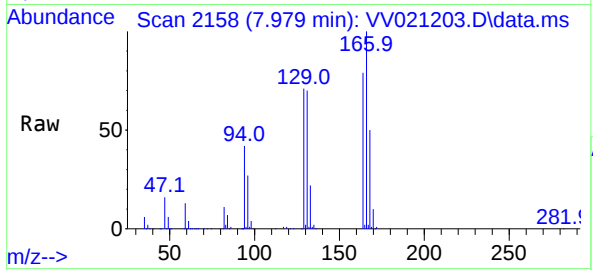

Tgt Ion:164	Resp:	347970
Ion	Ratio	Lower Upper
164	100	
129	88.9	63.8 118.4
131	87.8	59.3 110.1
166	126.0	87.7 162.9

