

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042821\
 Data File : VV021204.D
 Acq On : 28 Apr 2021 16:14
 Operator : SY/MD
 Sample : M2165-01ME
 Misc : 5.22g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB3E4ME

Quant Time: Apr 29 04:14:47 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 29 04:12:32 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	809766	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.860	117	821049	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.259	152	401921	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	237357	35.67	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	71.34%		
7) Chloroethane-d5	1.568	69	170690	34.87	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	69.74%#		
11) 1,1-Dichloroethene-d2	2.089	63	310096	25.27	ug/L	-0.02
Spiked Amount 50.000	Range 60 - 125		Recovery =	50.54%#		
21) 2-Butanone-d5	3.912	46	198789	61.18	ug/L	0.01
Spiked Amount 100.000	Range 40 - 130		Recovery =	61.18%		
24) Chloroform-d	4.349	84	477963	40.29	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	80.58%		
26) 1,2-Dichloroethane-d4	5.034	65	304308	40.36	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	80.72%		
32) Benzene-d6	5.047	84	942471	43.10	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	86.20%		
36) 1,2-Dichloropropane-d6	6.072	67	287792	44.09	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	88.18%		
41) Toluene-d8	7.320	98	873807	41.29	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	82.58%		
43) trans-1,3-Dichloroprop...	7.629	79	142777	40.03	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	80.06%		
47) 2-Hexanone-d5	8.127	63	232445	89.79	ug/L	0.04
Spiked Amount 100.000	Range 45 - 130		Recovery =	89.79%		
56) 1,1,2,2-Tetrachloroeth...	10.230	84	397462	40.37	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	80.74%		
66) 1,2-Dichlorobenzene-d4	11.635	152	375233	47.26	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	94.52%		
Target Compounds						
					Qvalue	
46) Tetrachloroethene	7.979	164	1305532	230.43	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042821\
Data File : VV021204.D
Acq On : 28 Apr 2021 16:14
Operator : SY/MD
Sample : M2165-01ME
Misc : 5.22g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB3E4ME

Quant Time: Apr 29 04:14:47 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 29 04:12:32 2021
Response via : Initial Calibration

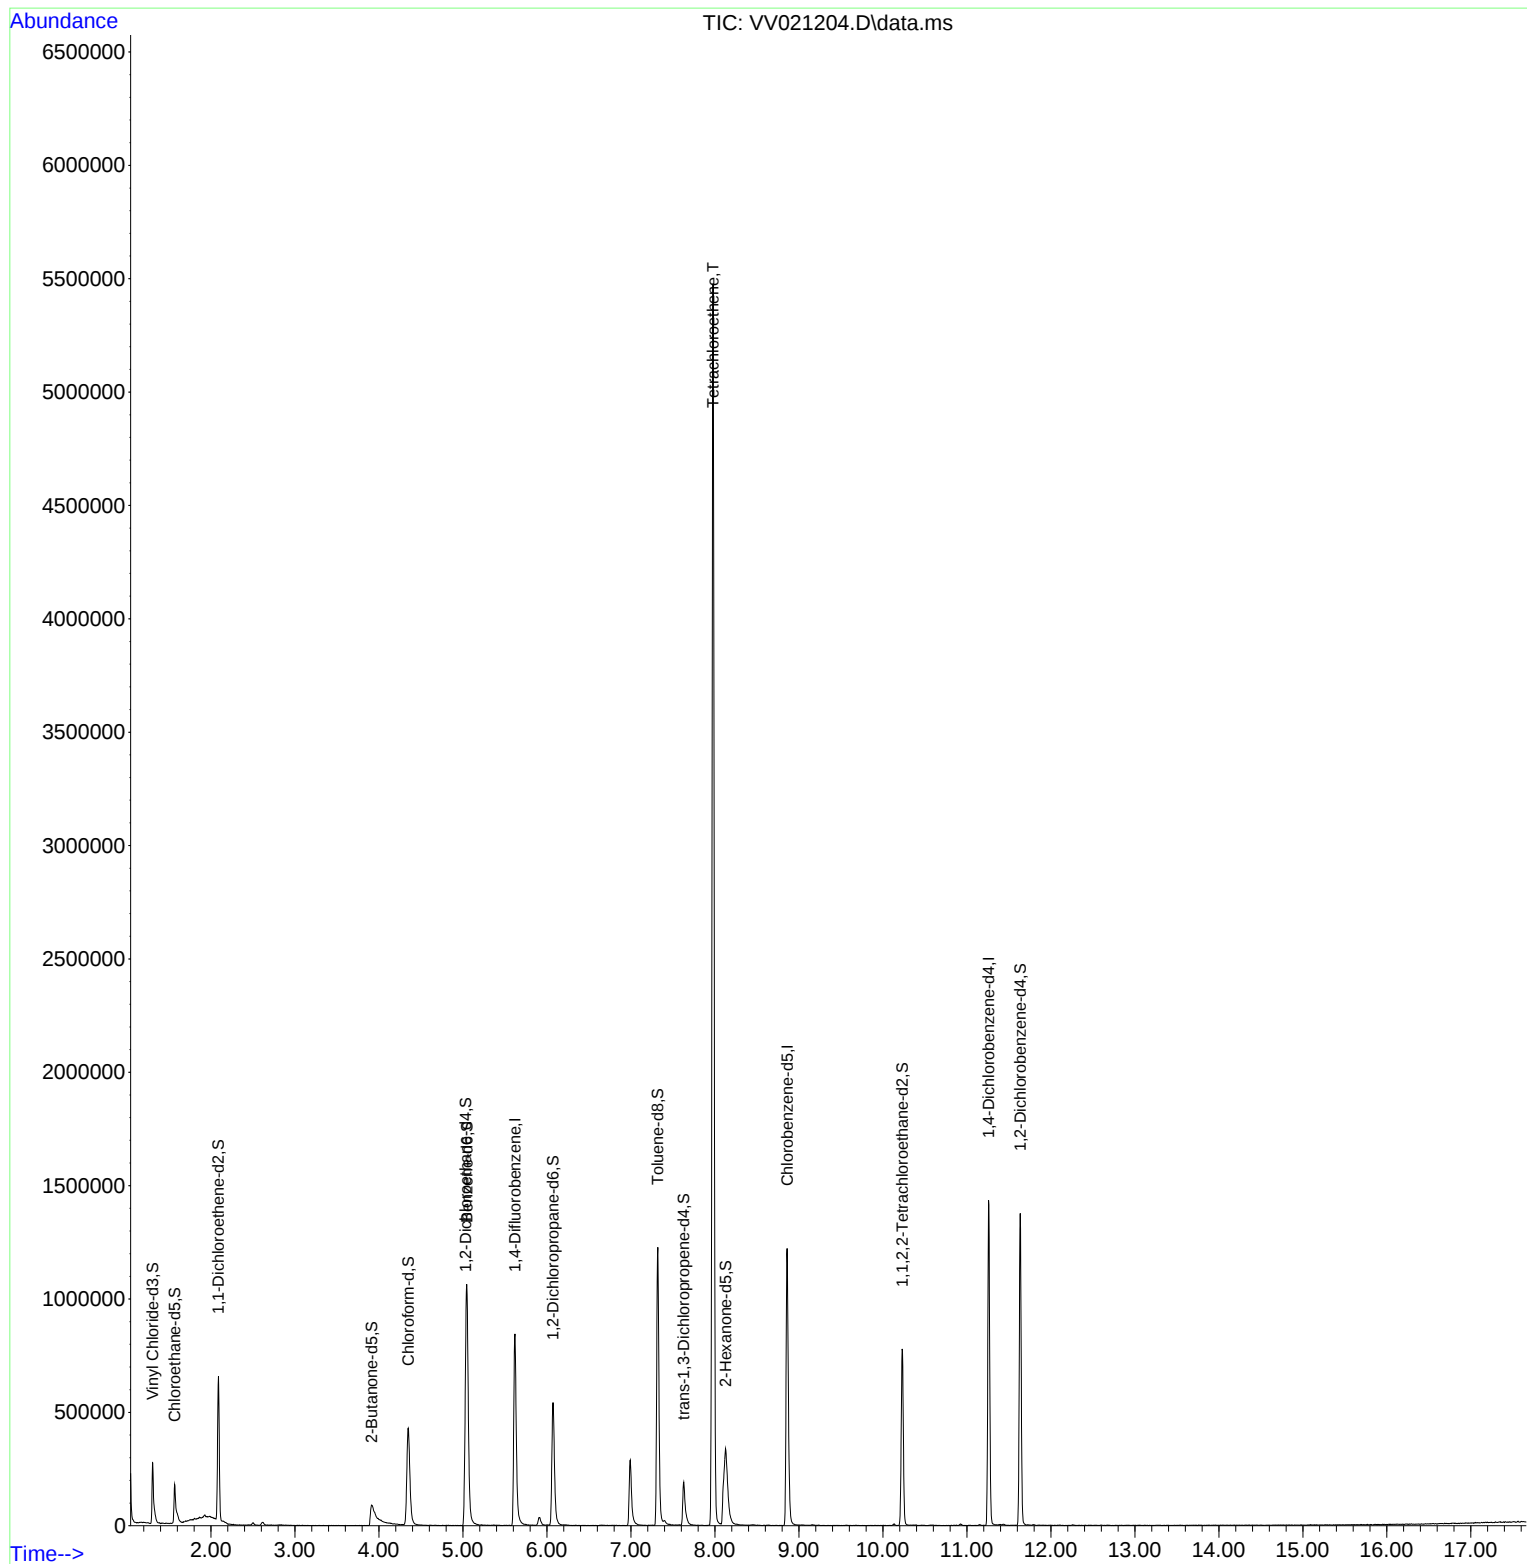

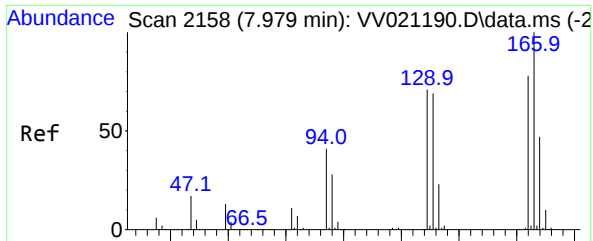

#46
Tetrachloroethene
Concen: 230.43 ug/L
RT: 7.979 min Scan# 2158
Delta R.T. 0.000 min
Lab File: VV021204.D
Acq: 28 Apr 2021 16:14

Instrument :
MSVOA_V
ClientSampleId :
GB3E4ME

Tgt Ion:164 Resp: 1305532
Ion Ratio Lower Upper
164 100
129 91.3 63.8 118.4
131 87.5 59.3 110.1
166 129.2 87.7 162.9

