

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042821\
 Data File : VW021205.D
 Acq On : 28 Apr 2021 16:37
 Operator : SY/MD
 Sample : M2181-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7C1

Manual Integrations
 APPROVED

MMDadoda
 4/30/2021 11:13:50 AM

Quant Time: Apr 29 04:14:53 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 29 04:12:32 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	762371	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	756830	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.255	152	369688	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	220043	35.13	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	70.26%		
7) Chloroethane-d5	1.568	69	185214	40.19	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	80.38%		
11) 1,1-Dichloroethene-d2	2.108	63	318160	27.54	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	55.08%#		
21) 2-Butanone-d5	3.902	46	294607	96.31	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	96.31%		
24) Chloroform-d	4.352	84	459748	41.17	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	82.34%		
26) 1,2-Dichloroethane-d4	5.034	65	294999	41.55	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	83.10%		
32) Benzene-d6	5.053	84	893955	44.35	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	88.70%		
36) 1,2-Dichloropropane-d6	6.072	67	283784	47.17	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	94.34%		
41) Toluene-d8	7.320	98	840527	43.09	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	86.18%		
43) trans-1,3-Dichloroprop...	7.625	79	134913	41.03	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	82.06%		
47) 2-Hexanone-d5	8.095	63	204847	85.84	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	85.84%		
56) 1,1,2,2-Tetrachloroeth...	10.223	84	365935	40.32	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	80.64%		
66) 1,2-Dichlorobenzene-d4	11.631	152	360593	49.38	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	98.76%		
Target Compounds					Qvalue	
13) Acetone	2.188	43	16728m	5.85	ug/L	
46) Tetrachloroethene	7.985	164	6769	1.30	ug/L	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042821\
Data File : VV021205.D
Acq On : 28 Apr 2021 16:37
Operator : SY/MD
Sample : M2181-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
BG7C1

Manual Integrations
APPROVED

MMDadoda
4/30/2021 11:13:50 AM


Quant Time: Apr 29 04:14:53 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 29 04:12:32 2021
Response via : Initial Calibration

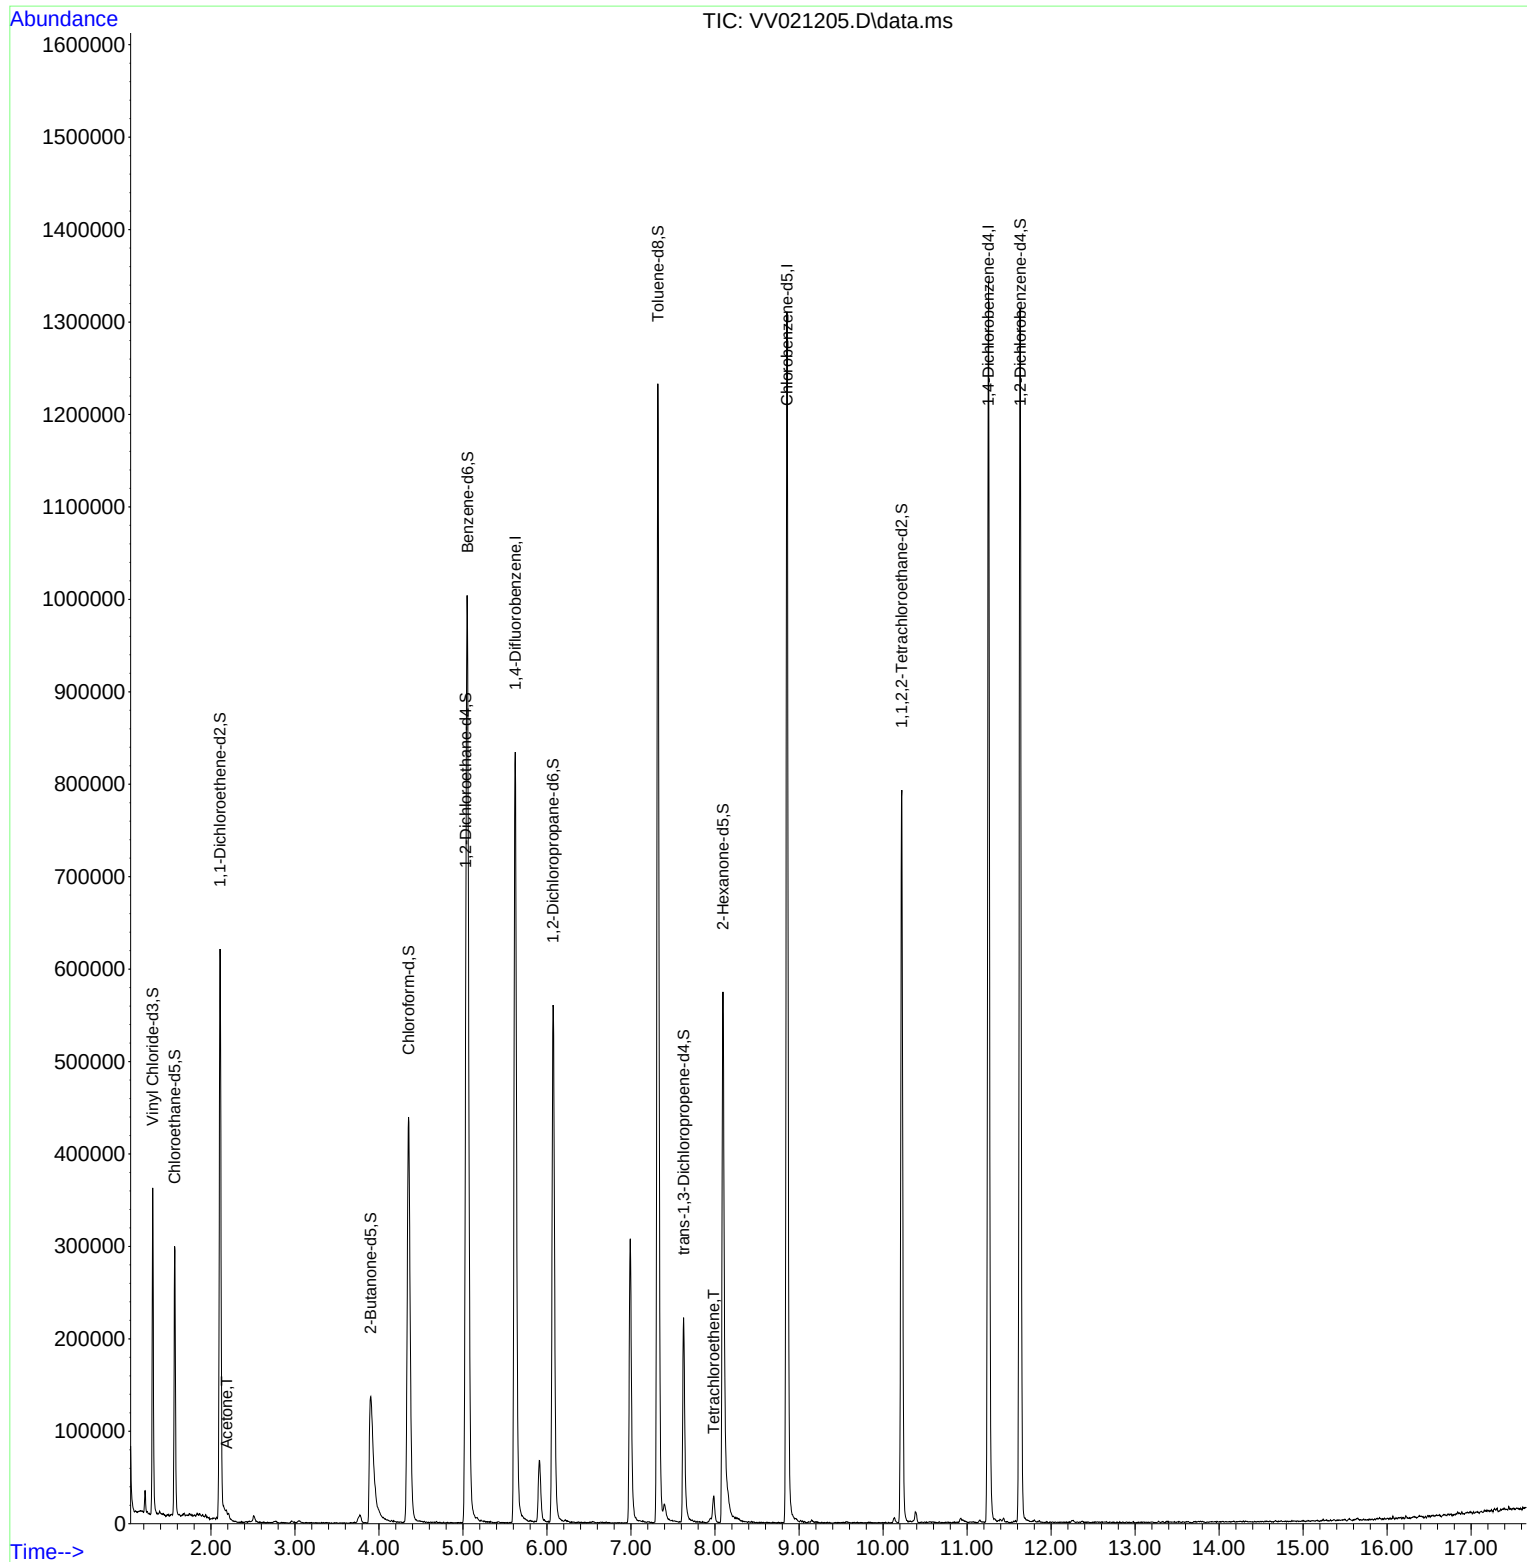

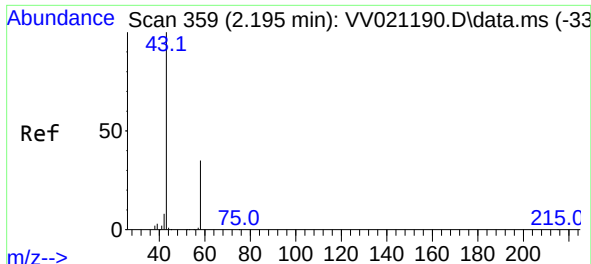

#13
Acetone
Concen: 5.85 ug/L m
RT: 2.188 min Scan# 357
Delta R.T. -0.007 min
Lab File: VV021205.D
Acq: 28 Apr 2021 16:37




Instrument :
MSVOA_V
ClientSampled :
BG7C1

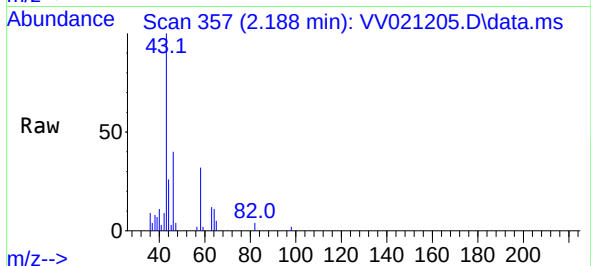


Tgt Ion: 43 Resp: 16728
Ion Ratio Lower Upper
43 100
58 10.7 0.0 30.8

Manual Integrations
APPROVED

MMDadoda
4/30/2021 11:13:50 AM

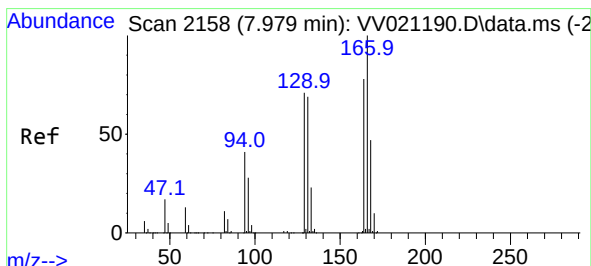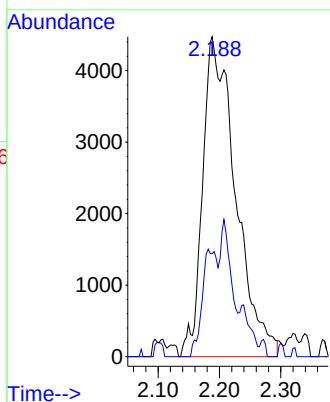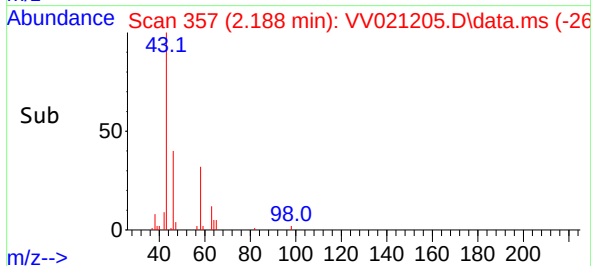

#46
Tetrachloroethene
Concen: 1.30 ug/L
RT: 7.985 min Scan# 2160
Delta R.T. 0.006 min
Lab File: VV021205.D
Acq: 28 Apr 2021 16:37

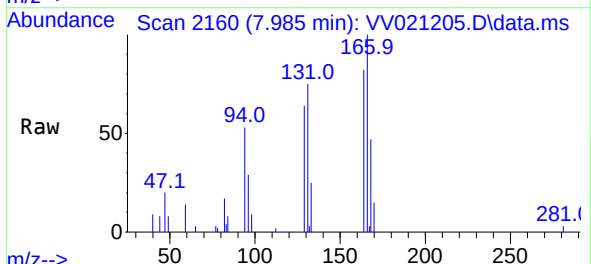

Tgt Ion: 164 Resp: 6769
Ion Ratio Lower Upper
164 100
129 77.9 63.8 118.4
131 92.1 59.3 110.1
166 122.0 87.7 162.9

