

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042821\
 Data File : VW021210.D
 Acq On : 28 Apr 2021 18:59
 Operator : SY/MD
 Sample : M2166-05ME
 Misc : 5.7g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB3G8ME

Quant Time: Apr 29 04:15:34 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 29 04:12:32 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	778840	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	788060	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.255	152	385222	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	222745	34.81	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	69.62%		
7) Chloroethane-d5	1.568	69	194461	41.30	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	82.60%		
11) 1,1-Dichloroethene-d2	2.108	63	322210	27.30	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	54.60%#		
21) 2-Butanone-d5	3.896	46	307418	98.37	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	98.37%		
24) Chloroform-d	4.352	84	481858	42.23	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	84.46%		
26) 1,2-Dichloroethane-d4	5.034	65	304881	42.04	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	84.08%		
32) Benzene-d6	5.053	84	917674	43.72	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	87.44%		
36) 1,2-Dichloropropane-d6	6.072	67	289461	46.21	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	92.42%		
41) Toluene-d8	7.320	98	877810	43.22	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	86.44%		
43) trans-1,3-Dichloroprop...	7.625	79	142733	41.69	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	83.38%		
47) 2-Hexanone-d5	8.095	63	226501	91.16	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	91.16%		
56) 1,1,2,2-Tetrachloroeth...	10.220	84	404705	42.83	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	85.66%		
66) 1,2-Dichlorobenzene-d4	11.632	152	380899	50.06	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	100.12%		
Target Compounds						Qvalue
46) Tetrachloroethene	7.982	164	26234	4.82	ug/L	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042821\
Data File : VV021210.D
Acq On : 28 Apr 2021 18:59
Operator : SY/MD
Sample : M2166-05ME
Misc : 5.7g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB3G8ME

Quant Time: Apr 29 04:15:34 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 29 04:12:32 2021
Response via : Initial Calibration

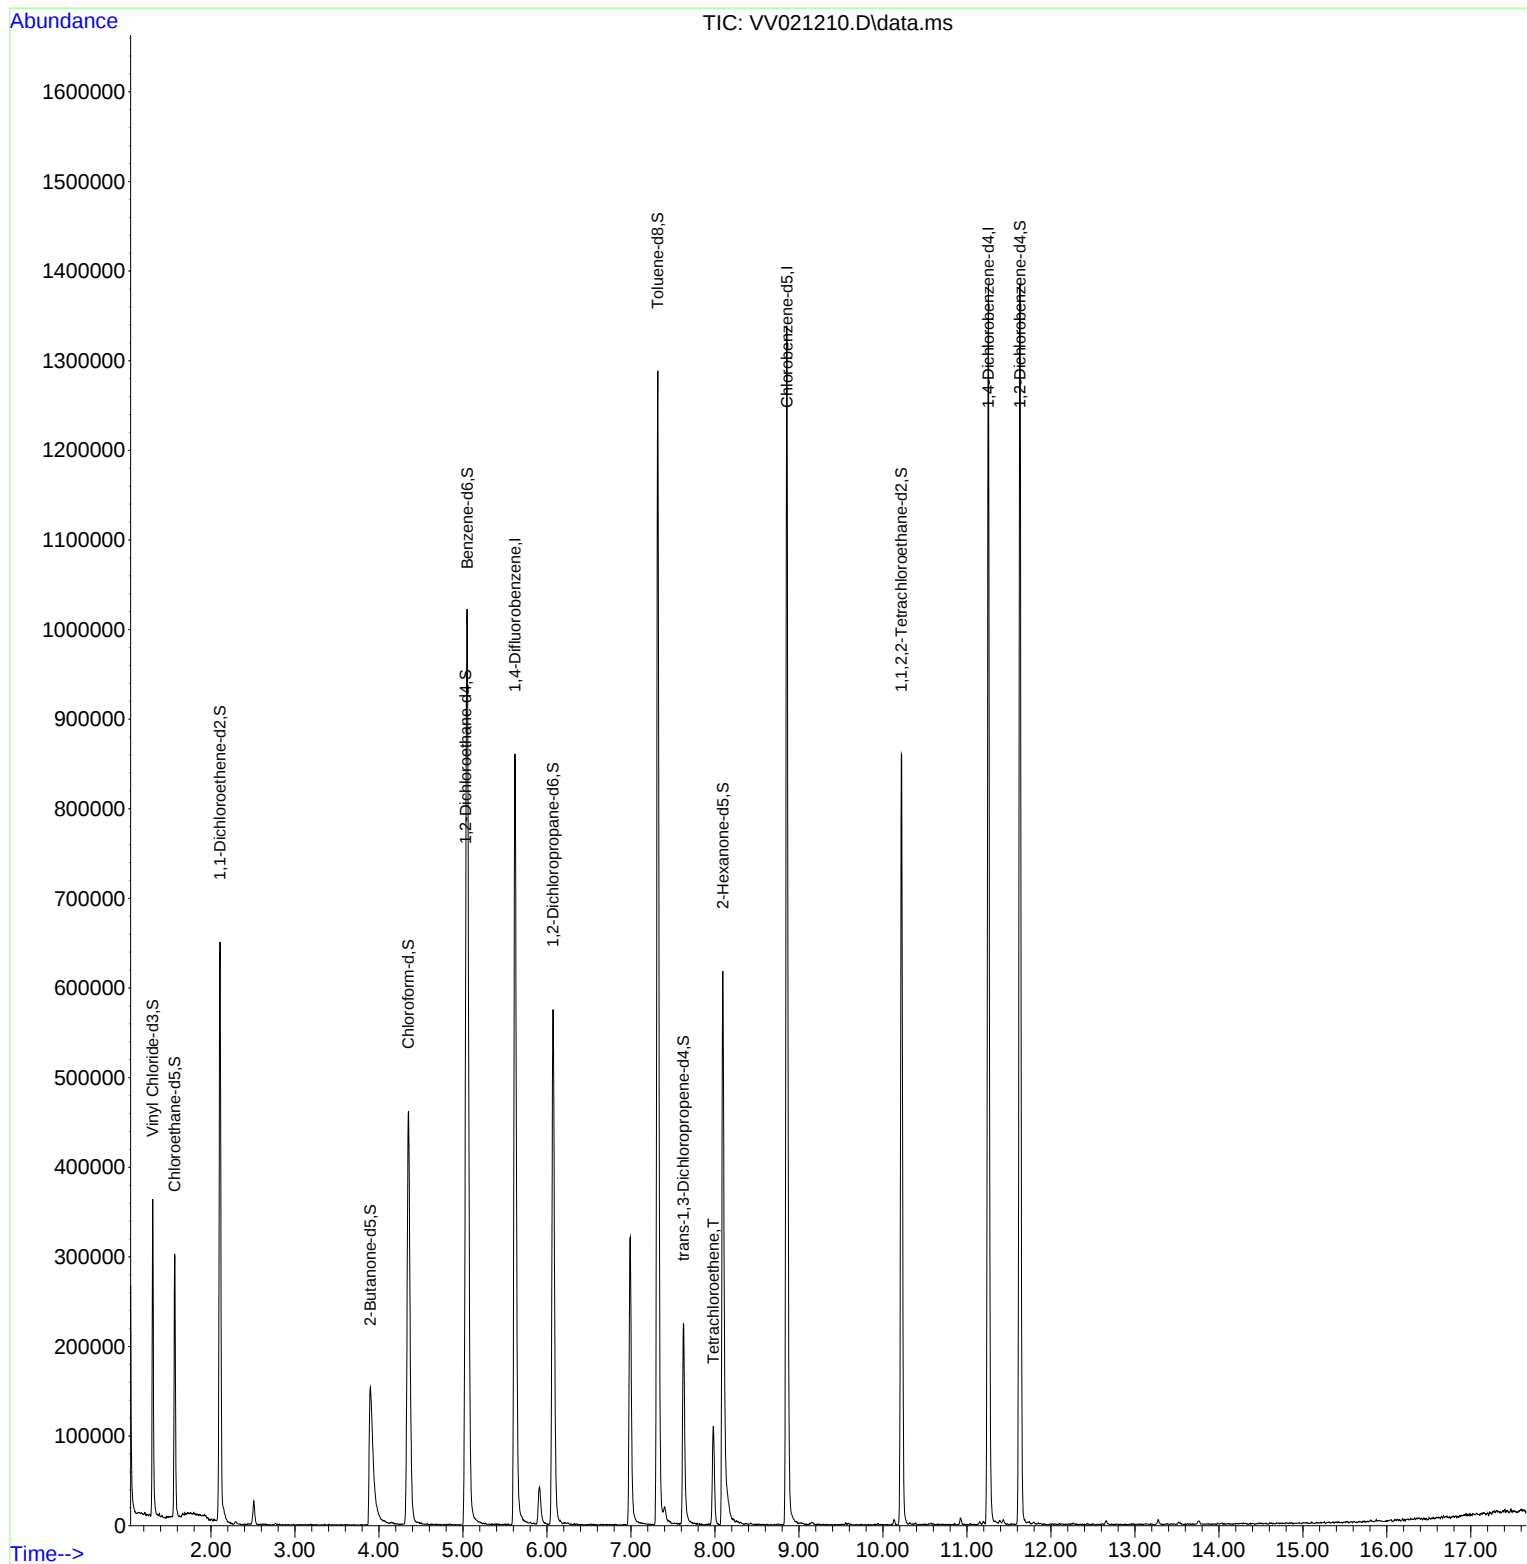

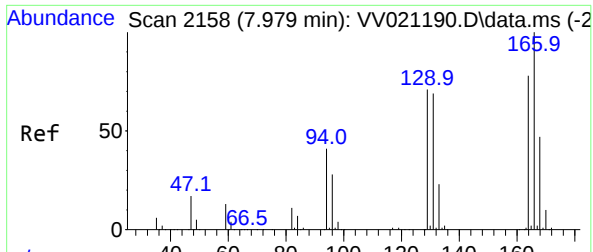

#46
Tetrachloroethene
Concen: 4.82 ug/L
RT: 7.982 min Scan# 2159
Delta R.T. 0.003 min
Lab File: VV021210.D
Acq: 28 Apr 2021 18:59

Instrument :
MSVOA_V
ClientSampleId :
GB3G8ME

Tgt Ion:164 Resp: 26234

Ion	Ratio	Lower	Upper
164	100		
129	95.6	63.8	118.4
131	97.3	59.3	110.1
166	149.5	87.7	162.9

