

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042821\
 Data File : VW021215.D
 Acq On : 28 Apr 2021 20:55
 Operator : SY/MD
 Sample : BLK
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK20

Quant Time: Apr 29 04:16:07 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 29 04:12:32 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.648	114	127	50.00	ug/L	# 0.03
28) Chlorobenzene-d5	8.873	117	2161	50.00	ug/L	# 0.02
58) 1,4-Dichlorobenzene-d4	11.265	152	3281	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	892	854.77	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	= 1709.54%#	
7) Chloroethane-d5	1.574	69	104	135.47	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	= 270.94%#	
11) 1,1-Dichloroethene-d2	2.111	63	1403	728.92	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	= 1457.84%#	
21) 2-Butanone-d5	4.175	46	92	180.54	ug/L	0.28
Spiked Amount	100.000	Range	40 - 130	Recovery	= 180.54%#	
24) Chloroform-d	4.365	84	382	205.33	ug/L	0.02
Spiked Amount	50.000	Range	70 - 125	Recovery	= 410.66%#	
26) 1,2-Dichloroethane-d4	5.053	65	132	111.62	ug/L	0.02
Spiked Amount	50.000	Range	70 - 125	Recovery	= 223.24%#	
32) Benzene-d6	5.088	84	321	5.58	ug/L	0.04
Spiked Amount	50.000	Range	70 - 125	Recovery	= 11.16%#	
36) 1,2-Dichloropropane-d6	6.098	67	91	5.30	ug/L	0.03
Spiked Amount	50.000	Range	70 - 120	Recovery	= 10.60%#	
41) Toluene-d8	7.342	98	1343	24.11	ug/L	0.03
Spiked Amount	50.000	Range	80 - 120	Recovery	= 48.22%#	
43) trans-1,3-Dichloroprop...	7.658	79	178	18.96	ug/L	0.04
Spiked Amount	50.000	Range	60 - 125	Recovery	= 37.92%#	
47) 2-Hexanone-d5	0.000	63	0	0.00	ug/L	
Spiked Amount	100.000	Range	45 - 130	Recovery	= 0.00%#	
56) 1,1,2,2-Tetrachloroeth...	10.223	84	388	14.97	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	= 29.94%#	
66) 1,2-Dichlorobenzene-d4	11.638	152	2132	32.90	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	= 65.80%#	
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	1.253	85	40	31.20	ug/L	# 42
3) Chloromethane	1.240	50	204	184.84	ug/L	# 42
5) Vinyl chloride	1.362	62	41	36.29	ug/L	# 1
6) Bromomethane	1.516	94	138	181.30	ug/L	95
8) Chloroethane	1.590	64	171	256.55	ug/L	86
9) Trichlorofluoromethane	1.751	101	77	38.25	ug/L	# 1
10) 1,1,2-Trichloro-1,2,2-...	2.130	101	47	47.07	ug/L	# 1
12) 1,1-Dichloroethene	2.092	96	192	211.77	ug/L	# 6
13) Acetone	2.108	43	473	993.70	ug/L	85
14) Carbon disulfide	2.294	76	708	284.68	ug/L	# 74
15) Methyl Acetate	2.462	43	149	189.27	ug/L	# 48
16) Methylene chloride	2.510	84	13981	14787.14	ug/L	81
18) Methyl tert-butyl Ether	3.018	73	45	16.83	ug/L	# 1
19) 1,1-Dichloroethane	3.121	63	51	32.44	ug/L	# 50
20) cis-1,2-Dichloroethene	3.754	96	45	48.40	ug/L	# 1
22) 2-Butanone	3.944	43	45	81.63	ug/L	# 49
25) Chloroform	4.384	83	145	81.95	ug/L	# 18
29) Cyclohexane	4.574	56	91	4.14	ug/L	# 66
31) Carbon tetrachloride	4.654	117	88	3.29	ug/L	# 3

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042821\
 Data File : VV021215.D
 Acq On : 28 Apr 2021 20:55
 Operator : SY/MD
 Sample : BLK
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK20


Quant Time: Apr 29 04:16:07 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 29 04:12:32 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

33) Benzene	5.095	78	41	0.68	ug/L	100
37) 1,2-Dichloropropane	6.394	63	44	2.97	ug/L #	85
38) Bromodichloromethane	6.465	83	87	3.77	ug/L #	24
40) 4-Methyl-2-pentanone	7.223	43	73	4.08	ug/L #	40
42) Toluene	7.416	91	60	0.91	ug/L #	22
44) trans-1,3-Dichloropropene	7.651	75	42	1.68	ug/L #	43
46) Tetrachloroethene	7.989	164	1638	109.84	ug/L	83
49) Dibromochloromethane	8.333	129	40	2.02	ug/L #	10
51) Chlorobenzene	8.915	112	49	1.08	ug/L #	31
54) o-Xylene	9.725	106	44	1.60	ug/L #	1
57) 1,1,2,2-Tetrachloroethane	10.513	83	47	1.84	ug/L #	25
61) 1,2,3-Trichloropropane	9.831	75	53	0.96	ug/L #	37
67) 1,2-Dichlorobenzene	11.657	146	82	0.81	ug/L #	25
69) 1,3,5-Trichlorobenzene	12.664	180	148	1.95	ug/L #	72
70) 1,2,4-trichlorobenzene	13.278	180	54	0.87	ug/L #	1
71) Naphthalene	13.513	128	154	0.89	ug/L #	69

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Apr 29 04:16:07 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 29 04:12:32 2021
Response via : Initial Calibration







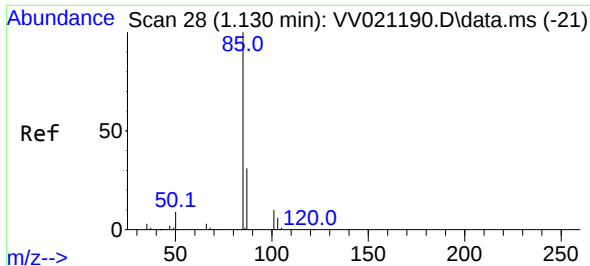

#2
Dichlorodifluoromethane
Concen: 31.20 ug/L
RT: 1.253 min Scan# 66
Delta R.T. 0.122 min
Lab File: VV021215.D
Acq: 28 Apr 2021 20:55




Instrument :
MSVOA_V
ClientSampleId :
VBLK20


Tgt Ion: 85 Resp: 40
Ion Ratio Lower Upper
85 100
87 0.0 25.8 38.8#

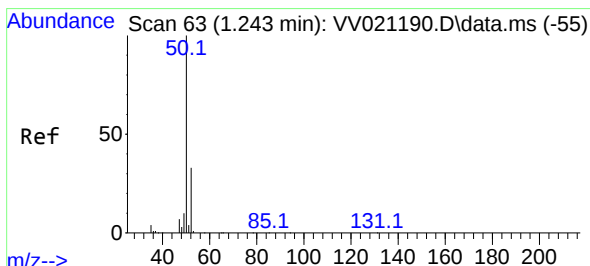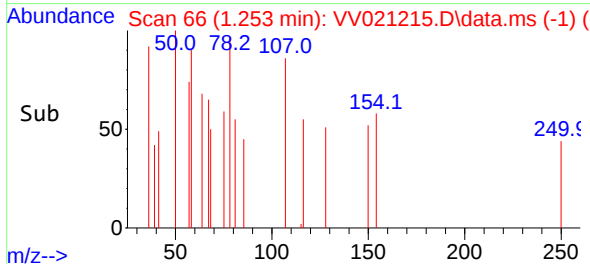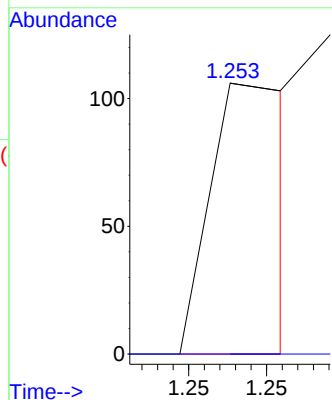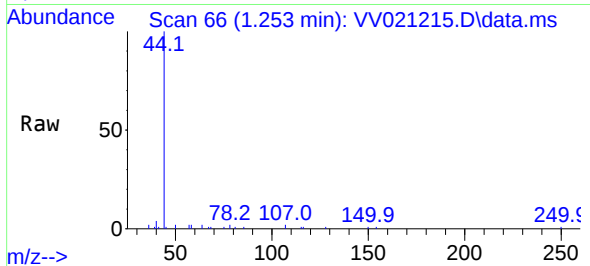

#3
Chloromethane
Concen: 184.84 ug/L
RT: 1.240 min Scan# 62
Delta R.T. -0.003 min
Lab File: VV021215.D
Acq: 28 Apr 2021 20:55

Tgt Ion: 50 Resp: 204
Ion Ratio Lower Upper
50 100
52 0.0 22.7 42.1#


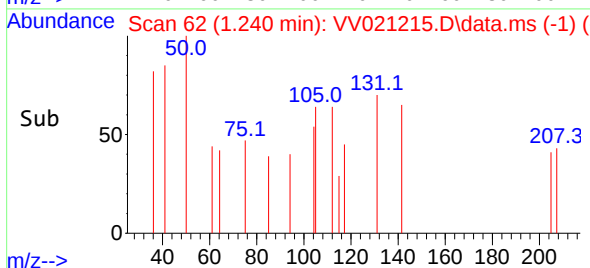
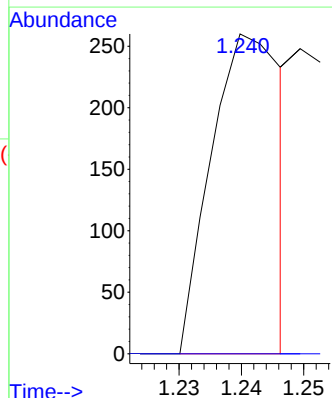
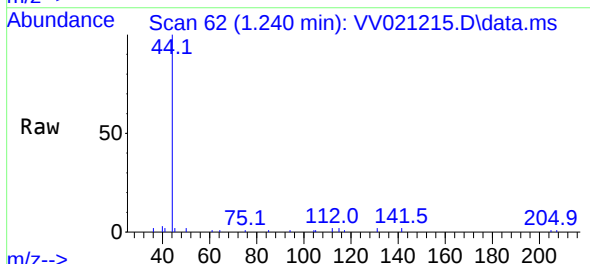


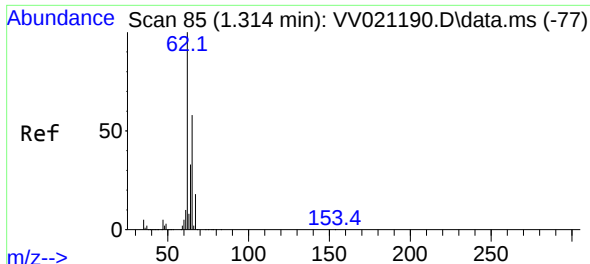

#5
 Vinyl chloride
 Concen: 36.29 ug/L
 RT: 1.362 min Scan# 100
 Delta R.T. 0.048 min
 Lab File: VV021215.D
 Acq: 28 Apr 2021 20:55




Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK20


Tgt Ion: 62 Resp: 41
 Ion Ratio Lower Upper
 62 100
 64 243.9 23.2 43.2#

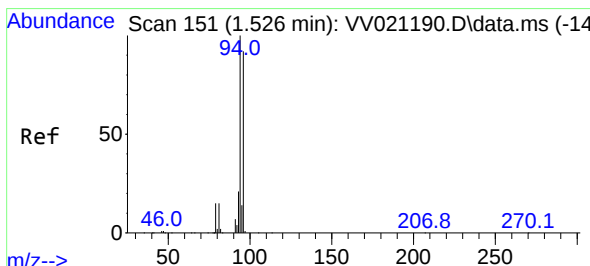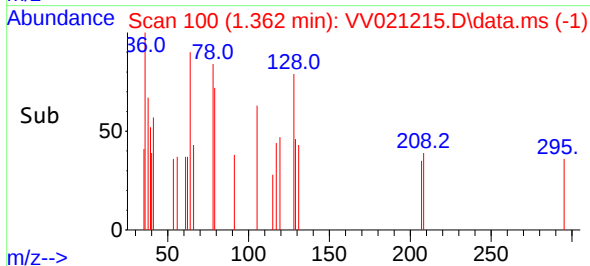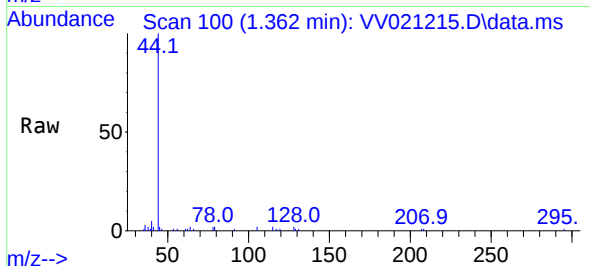

#6
 Bromomethane
 Concen: 181.30 ug/L
 RT: 1.516 min Scan# 148
 Delta R.T. -0.010 min
 Lab File: VV021215.D
 Acq: 28 Apr 2021 20:55

Tgt Ion: 94 Resp: 138
 Ion Ratio Lower Upper
 94 100
 96 98.3 65.7 122.1


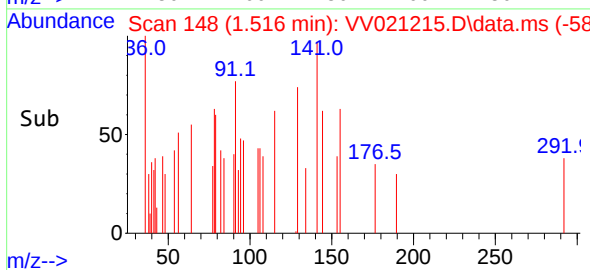

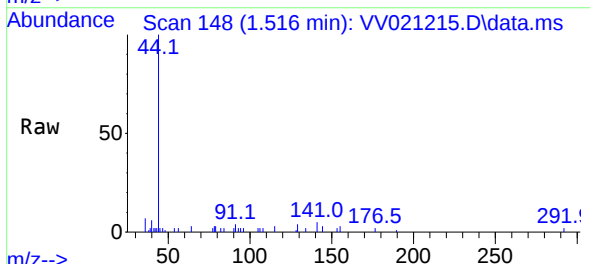




#8
Chloroethane
Concen: 256.55 ug/L
RT: 1.590 min Scan# 171
Delta R.T. 0.003 min
Lab File: VV021215.D
Acq: 28 Apr 2021 20:55




Instrument :
MSVOA_V
ClientSampleId :
VBLK20


Tgt Ion: 64 Resp: 171
Ion Ratio Lower Upper
64 100
66 41.9 23.7 43.9

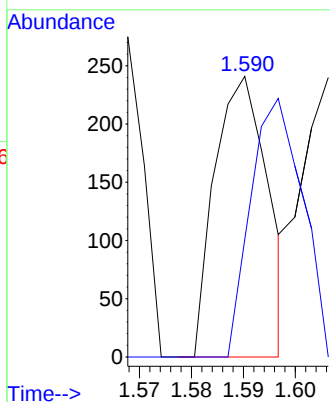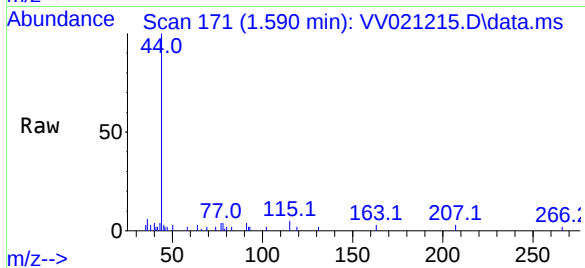

#9
Trichlorofluoromethane
Concen: 38.25 ug/L
RT: 1.751 min Scan# 221
Delta R.T. -0.003 min
Lab File: VV021215.D
Acq: 28 Apr 2021 20:55

Tgt Ion:101 Resp: 77
Ion Ratio Lower Upper
101 100
103 209.1 53.0 79.6#


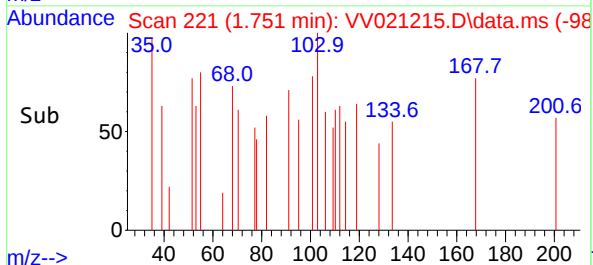

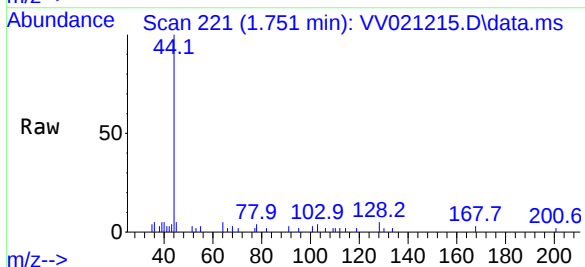




#10
1,1,2-Trichloro-1,2,2-trifluoroethane
Concen: 47.07 ug/L
RT: 2.130 min Scan# 339
Delta R.T. 0.013 min
Lab File: VV021215.D
Acq: 28 Apr 2021 20:55




Instrument :
MSVOA_V
ClientSampleId :
VBLK20


Tgt Ion:	101	Resp:	47
Ion	Ratio	Lower	Upper
101	100		
85	100.0	35.4	53.2#
151	197.9	63.9	95.9#

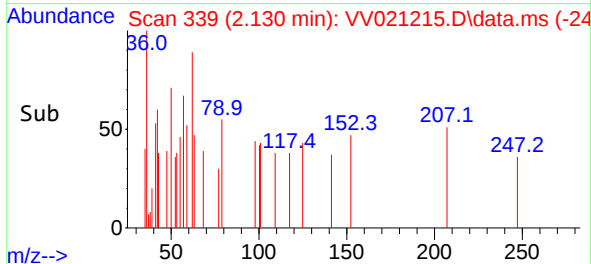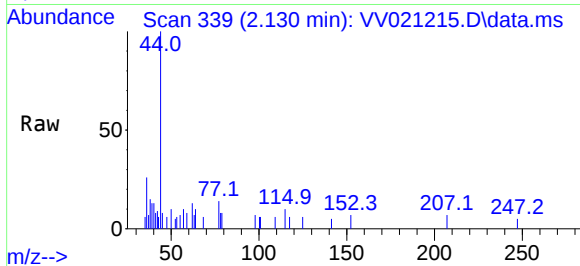

#12
1,1-Dichloroethene
Concen: 211.77 ug/L
RT: 2.092 min Scan# 327
Delta R.T. -0.029 min
Lab File: VV021215.D
Acq: 28 Apr 2021 20:55

Tgt Ion:	96	Resp:	192
Ion	Ratio	Lower	Upper
96	100		
61	0.0	121.4	225.6#
63	73.5	98.1	182.1#


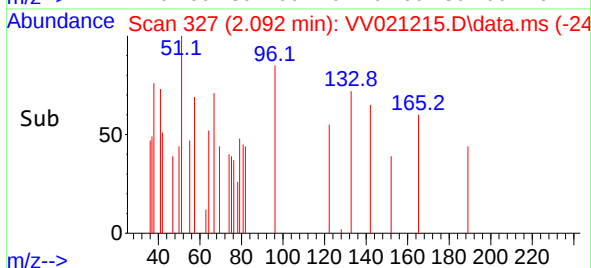
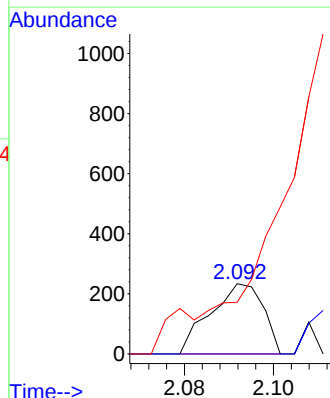
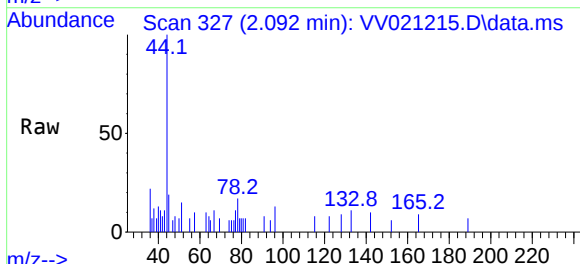


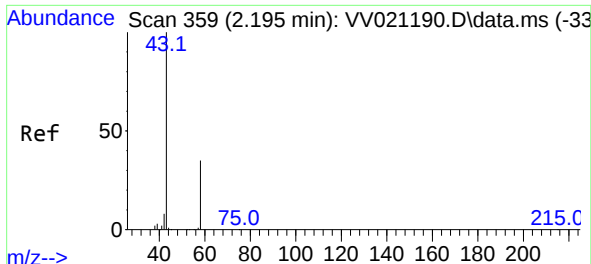

#13
Acetone
Concen: 993.70 ug/L
RT: 2.108 min Scan# 332
Delta R.T. -0.087 min
Lab File: VV021215.D
Acq: 28 Apr 2021 20:55




Instrument :
MSVOA_V
ClientSampleId :
VBLK20


Tgt Ion: 43 Resp: 473
Ion Ratio Lower Upper
43 100
58 9.3 0.0 30.8

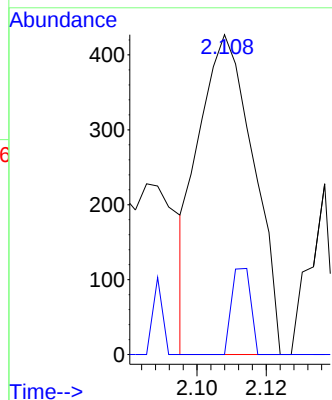

#14
Carbon disulfide
Concen: 284.68 ug/L
RT: 2.294 min Scan# 390
Delta R.T. -0.003 min
Lab File: VV021215.D
Acq: 28 Apr 2021 20:55

Tgt Ion: 76 Resp: 708
Ion Ratio Lower Upper
76 100
78 0.0 7.4 11.2#


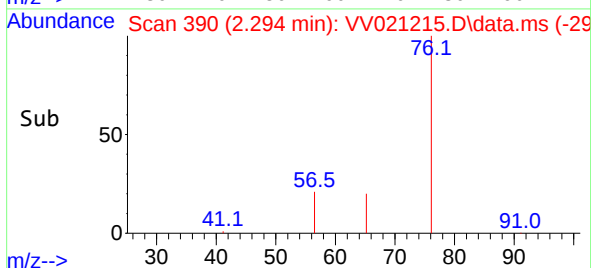
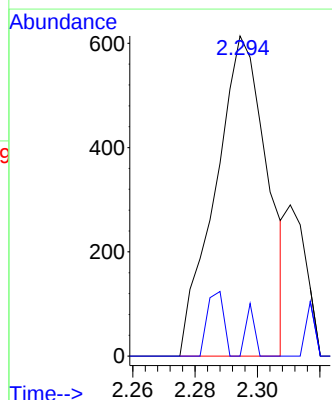
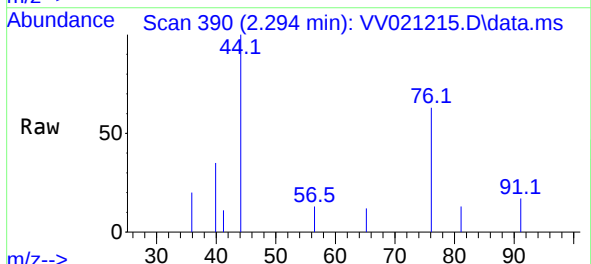




#15
Methyl Acetate
Concen: 189.27 ug/L
RT: 2.462 min Scan# 442
Delta R.T. 0.023 min
Lab File: VV021215.D
Acq: 28 Apr 2021 20:55




Instrument :
MSVOA_V
ClientSampleId :
VBLK20


Tgt Ion: 43 Resp: 149
Ion Ratio Lower Upper
43 100
74 0.0 21.2 31.8#

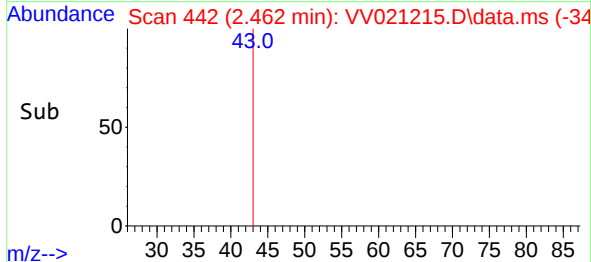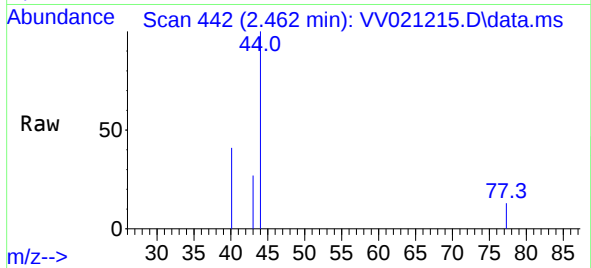

#16
Methylene chloride
Concen: 14787.14 ug/L
RT: 2.510 min Scan# 457
Delta R.T. 0.000 min
Lab File: VV021215.D
Acq: 28 Apr 2021 20:55

Tgt Ion: 84 Resp: 13981
Ion Ratio Lower Upper
84 100
86 51.3 44.9 83.5
49 90.4 78.1 145.1

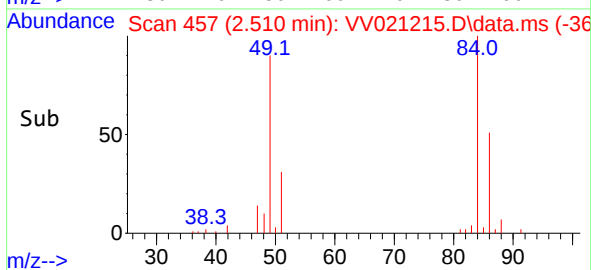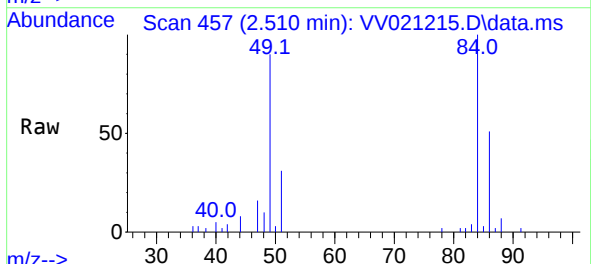







#18
Methyl tert-butyl Ether
Concen: 16.83 ug/L
RT: 3.018 min Scan# 615
Delta R.T. 0.248 min
Lab File: VV021215.D
Acq: 28 Apr 2021 20:55

Instrument :
MSVOA_V
ClientSampleId :
VBLK20

Tgt Ion: 73 Resp: 45




Ion	Ratio	Lower	Upper
73	100		
43	93.3	14.7	22.1#
57	0.0	15.9	23.9#

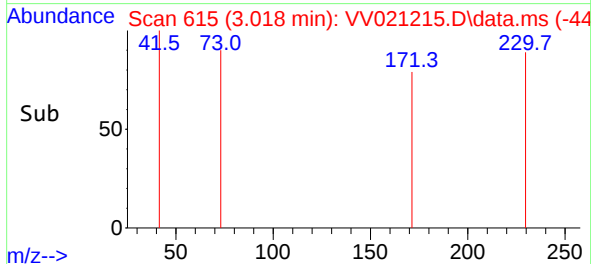


#19
1,1-Dichloroethane
Concen: 32.44 ug/L
RT: 3.121 min Scan# 647
Delta R.T. -0.071 min
Lab File: VV021215.D
Acq: 28 Apr 2021 20:55

Tgt Ion: 63 Resp: 51

Ion	Ratio	Lower	Upper
63	100		
65	0.0	21.9	40.7#
83	0.0	10.6	19.6#


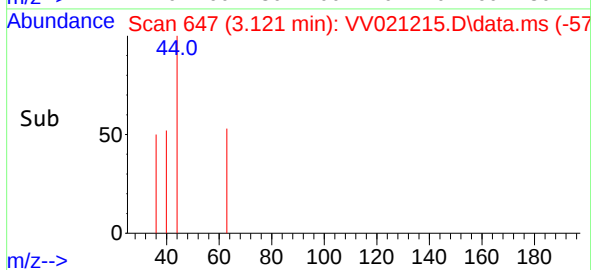

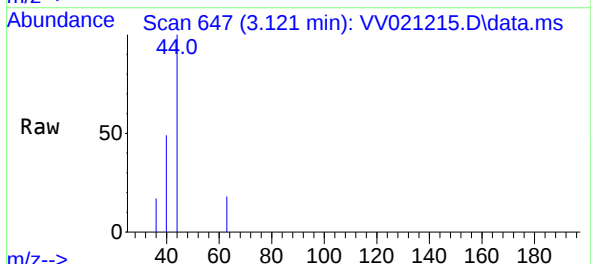




#20
cis-1,2-Dichloroethene
Concen: 48.40 ug/L
RT: 3.754 min Scan# 844
Delta R.T. -0.161 min
Lab File: VV021215.D
Acq: 28 Apr 2021 20:55




Instrument :
MSVOA_V
ClientSampleId :
VBLK20


Tgt Ion: 96 Resp: 45
Ion Ratio Lower Upper
96 100
61 0.0 84.4 156.7#
68 0.0 0.0 0.0

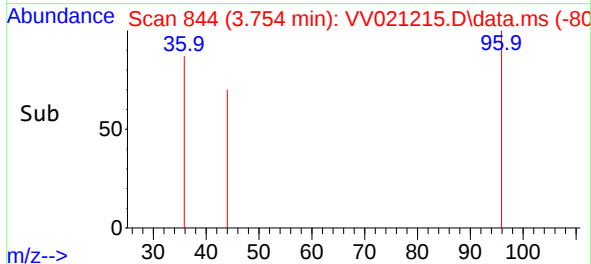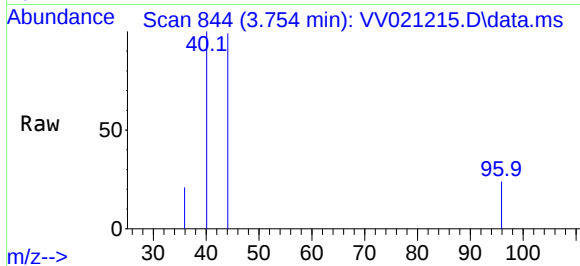

#22
2-Butanone
Concen: 81.63 ug/L
RT: 3.944 min Scan# 903
Delta R.T. -0.038 min
Lab File: VV021215.D
Acq: 28 Apr 2021 20:55

Tgt Ion: 43 Resp: 45
Ion Ratio Lower Upper
43 100
72 0.0 13.2 39.6#


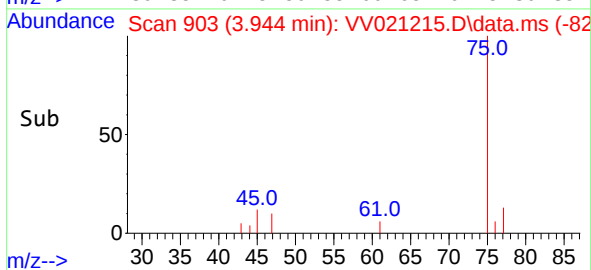

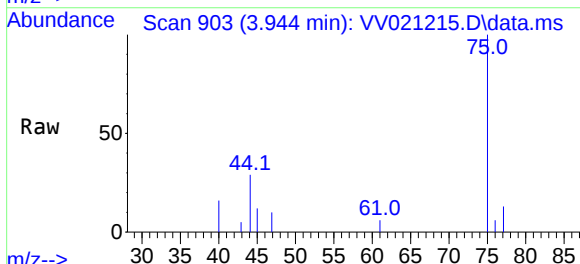




#25
Chloroform
Concen: 81.95 ug/L
RT: 4.384 min Scan# 1040
Delta R.T. 0.010 min
Lab File: VV021215.D
Acq: 28 Apr 2021 20:55




Instrument :
MSVOA_V
ClientSampleId :
VBLK20


Tgt Ion: 83 Resp: 145
Ion Ratio Lower Upper
83 100
85 0.0 45.6 84.6#

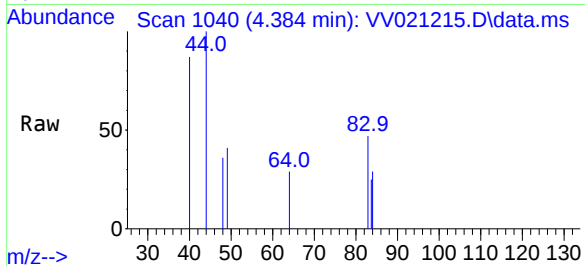

#29
Cyclohexane
Concen: 4.14 ug/L
RT: 4.574 min Scan# 1099
Delta R.T. -0.106 min
Lab File: VV021215.D
Acq: 28 Apr 2021 20:55

Tgt Ion: 56 Resp: 91
Ion Ratio Lower Upper
56 100
69 47.3 25.7 38.5#
84 59.3 75.7 113.5#


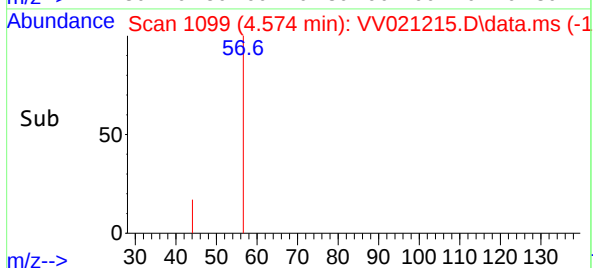
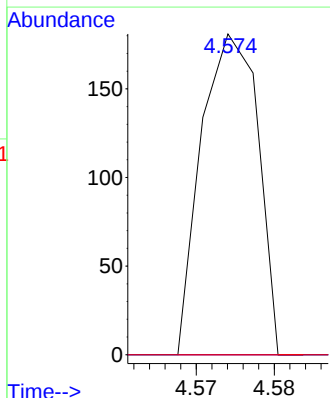
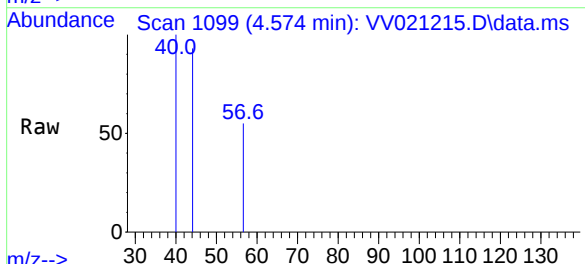




#31
Carbon tetrachloride
Concen: 3.29 ug/L
RT: 4.654 min Scan# 1124
Delta R.T. -0.173 min
Lab File: VV021215.D
Acq: 28 Apr 2021 20:55




Instrument :
MSVOA_V
ClientSampleId :
VBLK20


Tgt Ion:117 Resp: 88
Ion Ratio Lower Upper
117 100
119 0.0 75.4 113.2#

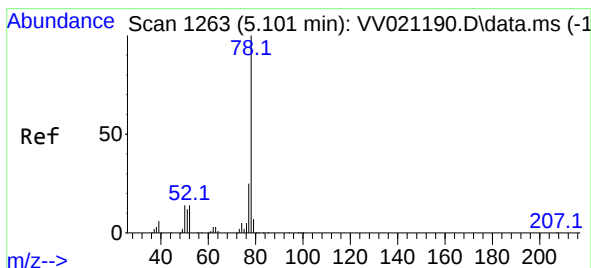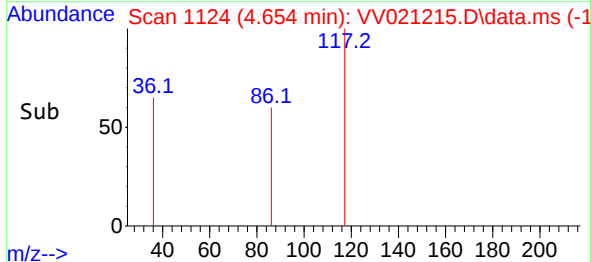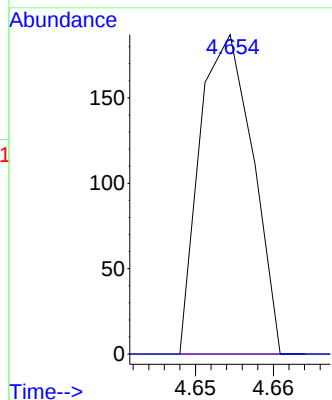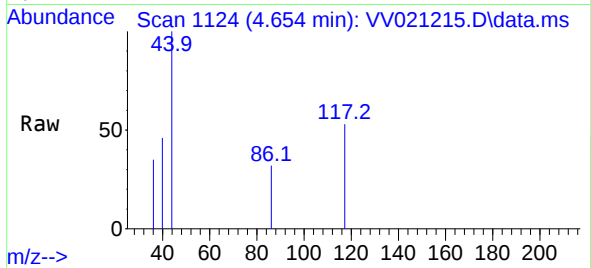

#33
Benzene
Concen: 0.68 ug/L
RT: 5.095 min Scan# 1261
Delta R.T. -0.006 min
Lab File: VV021215.D
Acq: 28 Apr 2021 20:55

Tgt Ion: 78 Resp: 41


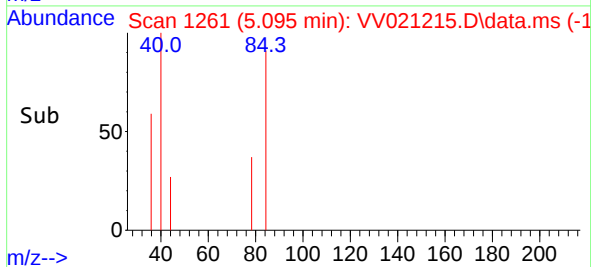
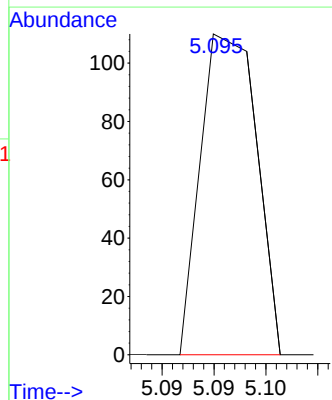
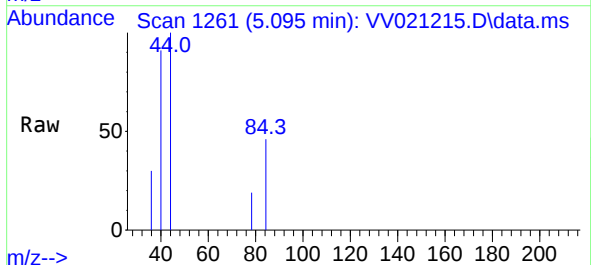




#37
1,2-Dichloropropane
Concen: 2.97 ug/L
RT: 6.394 min Scan# 1665
Delta R.T. 0.219 min
Lab File: VV021215.D
Acq: 28 Apr 2021 20:55




Instrument :
MSVOA_V
ClientSampleId :
VBLK20


Tgt Ion: 63 Resp: 44
Ion Ratio Lower Upper
63 100
112 0.0 3.9 5.9#

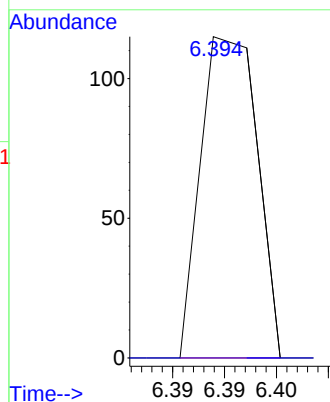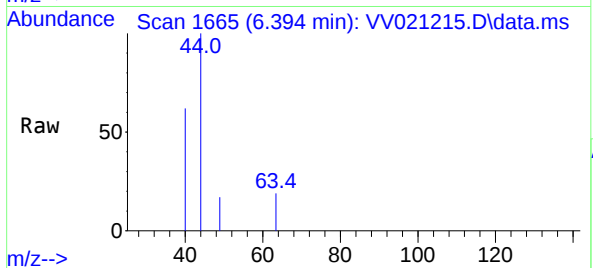

#38
Bromodichloromethane
Concen: 3.77 ug/L
RT: 6.465 min Scan# 1687
Delta R.T. -0.045 min
Lab File: VV021215.D
Acq: 28 Apr 2021 20:55

Tgt Ion: 83 Resp: 87
Ion Ratio Lower Upper
83 100
85 0.0 46.2 85.8#
127 0.0 7.4 11.0#

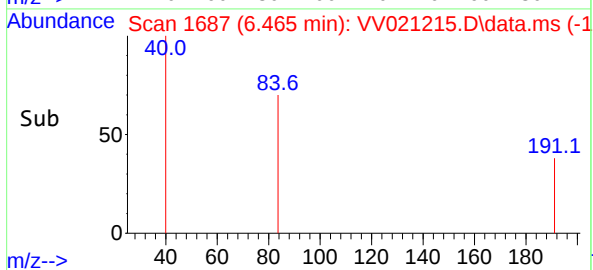







#40
4-Methyl-2-pentanone
Concen: 4.08 ug/L
RT: 7.223 min Scan# 1923
Delta R.T. -0.003 min
Lab File: VV021215.D
Acq: 28 Apr 2021 20:55

Instrument :
MSVOA_V
ClientSampleId :
VBLK20

Tgt Ion: 43 Resp: 73




Ion	Ratio	Lower	Upper
43	100		
58	0.0	34.5	51.7#
100	0.0	15.2	22.8#

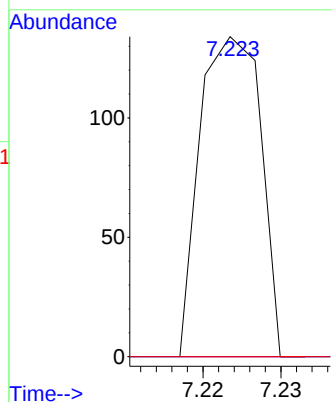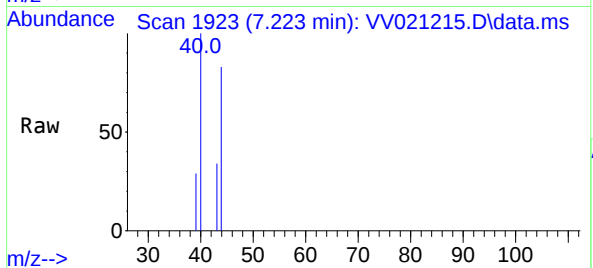


#42
Toluene
Concen: 0.91 ug/L
RT: 7.416 min Scan# 1983
Delta R.T. 0.026 min
Lab File: VV021215.D
Acq: 28 Apr 2021 20:55

Tgt Ion: 91 Resp: 60

Ion	Ratio	Lower	Upper
91	100		
92	0.0	41.0	76.2#


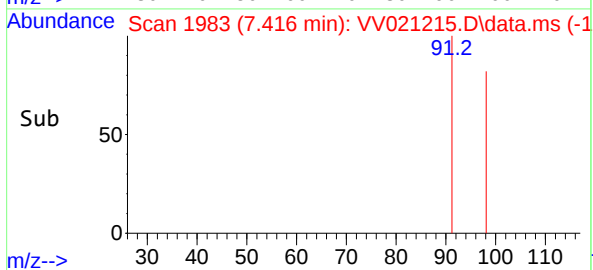
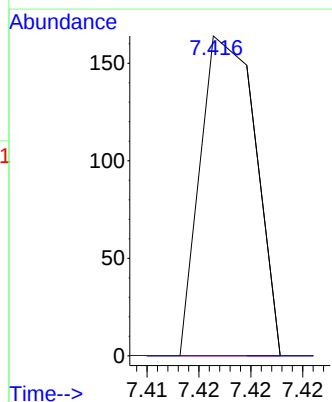





#44
trans-1,3-Dichloropropene
Concen: 1.68 ug/L
RT: 7.651 min Scan# 2056
Delta R.T. 0.000 min
Lab File: VV021215.D
Acq: 28 Apr 2021 20:55




Instrument :
MSVOA_V
ClientSampleId :
VBLK20


Tgt Ion: 75 Resp: 42
Ion Ratio Lower Upper
75 100
77 0.0 21.8 40.6#

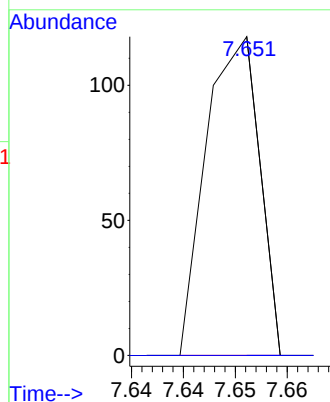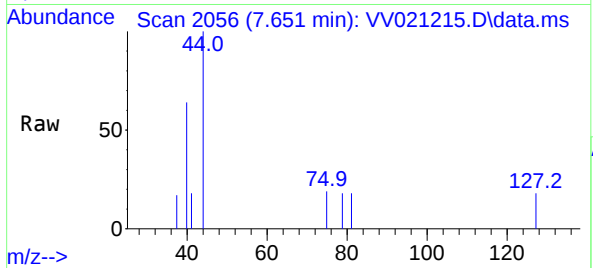

#46
Tetrachloroethene
Concen: 109.84 ug/L
RT: 7.989 min Scan# 2161
Delta R.T. 0.010 min
Lab File: VV021215.D
Acq: 28 Apr 2021 20:55

Tgt Ion:164 Resp: 1638
Ion Ratio Lower Upper
164 100
129 99.1 63.8 118.4
131 76.5 59.3 110.1
166 93.0 87.7 162.9

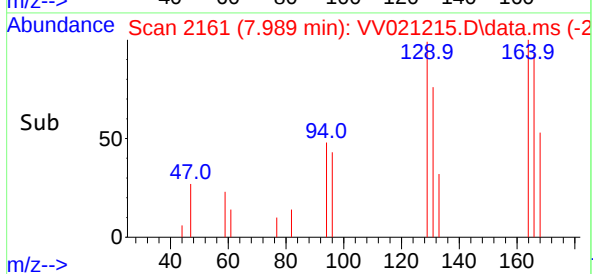



#49

Dibromochloromethane

Concen: 2.02 ug/L

RT: 8.333 min Scan# 2268





Delta R.T. 0.084 min

Lab File: VV021215.D

Acq: 28 Apr 2021 20:55

Tgt Ion:	129	Resp:	40
Ion Ratio	Lower	Upper	
129	100		
127	0.0	55.2	102.6#

Instrument :
MSVOA_V
ClientSampleId :
VBLK20

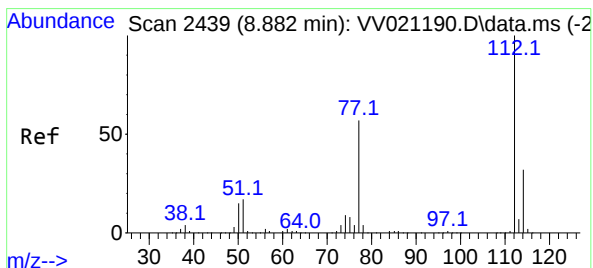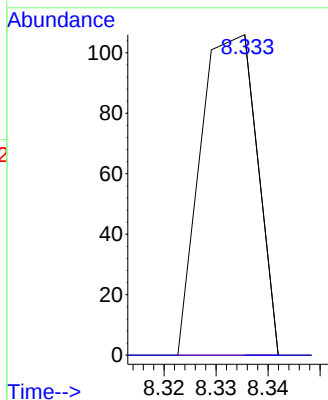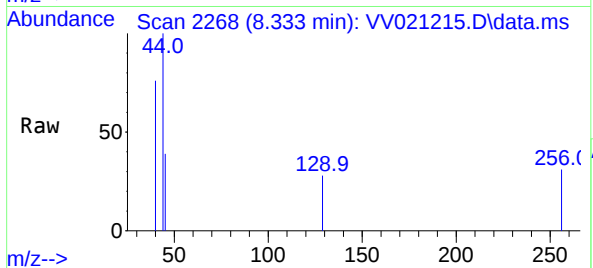

#51

Chlorobenzene

Concen: 1.08 ug/L




RT: 8.915 min Scan# 2449


Delta R.T. 0.032 min

Lab File: VV021215.D

Acq: 28 Apr 2021 20:55

Tgt Ion:	112	Resp:	49
Ion Ratio	Lower	Upper	
112	100		
114	0.0	22.8	42.4#
77	0.0	44.2	66.2#


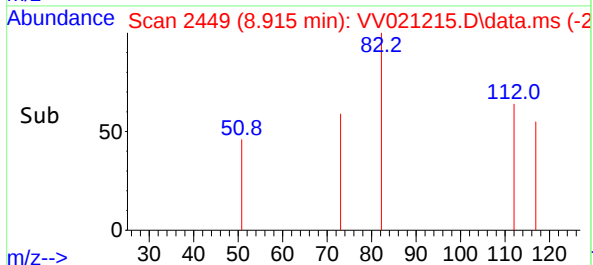
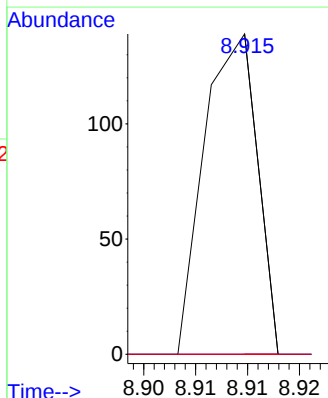
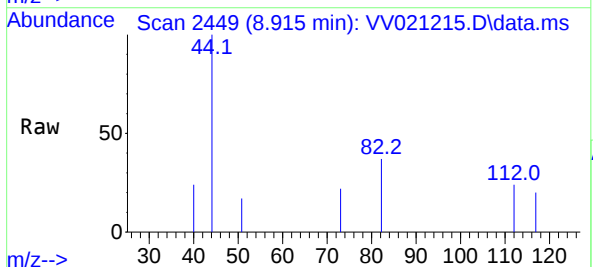




#54
o-Xylene
Concen: 1.60 ug/L
RT: 9.725 min Scan# 2701
Delta R.T. 0.177 min
Lab File: VV021215.D
Acq: 28 Apr 2021 20:55




Instrument :
MSVOA_V
ClientSampleId :
VBLK20


Tgt Ion:106 Resp: 44
Ion Ratio Lower Upper
106 100
91 0.0 150.4 279.4#

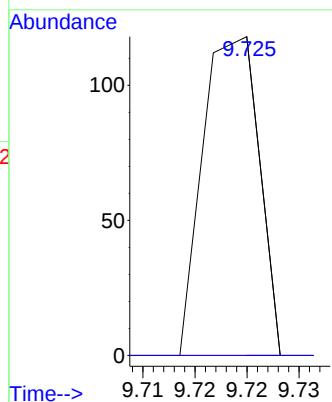

#57
1,1,2,2-Tetrachloroethane
Concen: 1.84 ug/L
RT: 10.513 min Scan# 2946
Delta R.T. 0.267 min
Lab File: VV021215.D
Acq: 28 Apr 2021 20:55

Tgt Ion: 83 Resp: 47
Ion Ratio Lower Upper
83 100
85 0.0 45.8 85.0#
131 0.0 8.8 13.2#


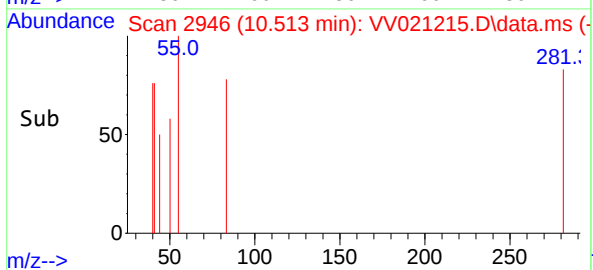
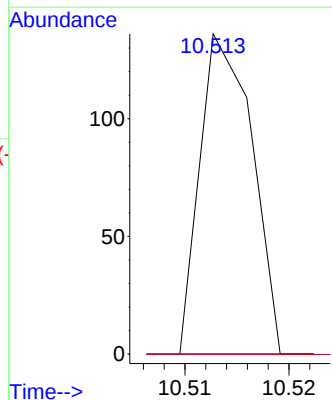





#61
1,2,3-Trichloropropane
Concen: 0.96 ug/L
RT: 9.831 min Scan# 2734
Delta R.T. -0.447 min
Lab File: VV021215.D
Acq: 28 Apr 2021 20:55




Instrument :
MSVOA_V
ClientSampleId :
VBLK20


Tgt Ion:	75	Resp:	53
Ion	Ratio	Lower	Upper
75	100		
77	0.0	25.8	38.8#
110	0.0	34.9	52.3#

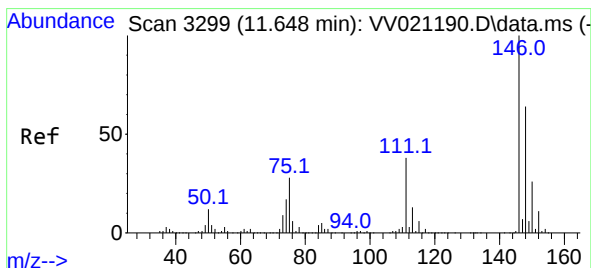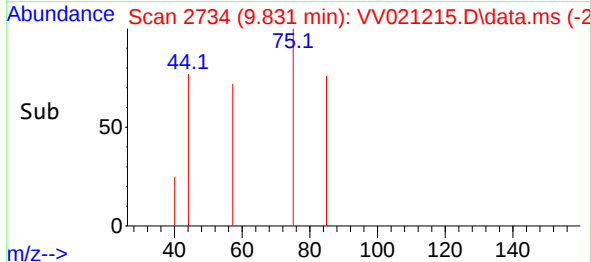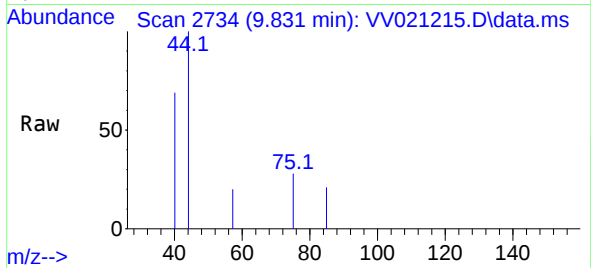

#67
1,2-Dichlorobenzene
Concen: 0.81 ug/L
RT: 11.657 min Scan# 3302
Delta R.T. 0.010 min
Lab File: VV021215.D
Acq: 28 Apr 2021 20:55

Tgt Ion:	146	Resp:	82
Ion	Ratio	Lower	Upper
146	100		
111	0.0	33.2	49.8#
148	0.0	50.6	75.8#


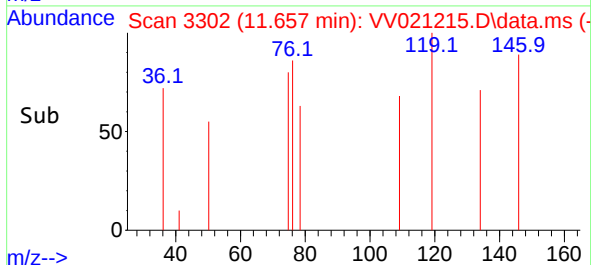
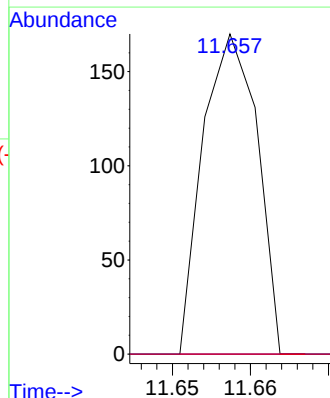
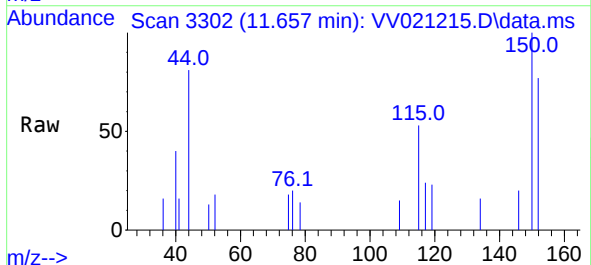


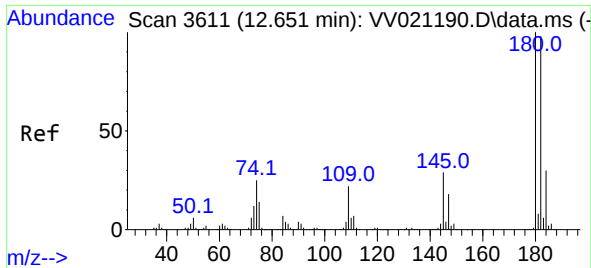

#69
1,3,5-Trichlorobenzene
Concen: 1.95 ug/L
RT: 12.664 min Scan# 3615
Delta R.T. 0.013 min
Lab File: VV021215.D
Acq: 28 Apr 2021 20:55




Instrument :
MSVOA_V
ClientSampleId :
VBLK20


Tgt Ion:	180	Resp:	148
Ion	Ratio	Lower	Upper
180	100		
182	69.6	77.4	116.0#
184	29.1	24.1	36.1
145	0.0	23.8	35.8#

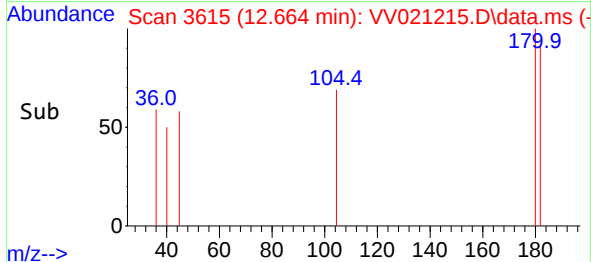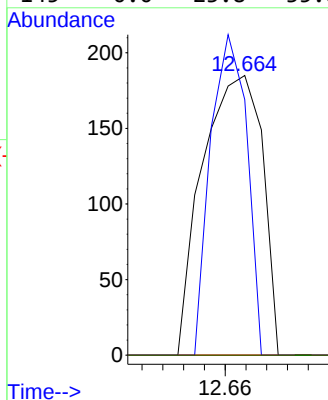

#70
1,2,4-trichlorobenzene
Concen: 0.87 ug/L
RT: 13.278 min Scan# 3806
Delta R.T. 0.010 min
Lab File: VV021215.D
Acq: 28 Apr 2021 20:55

Tgt Ion:	180	Resp:	54
Ion	Ratio	Lower	Upper
180	100		
182	0.0	77.5	116.3#
145	205.6	24.3	36.5#

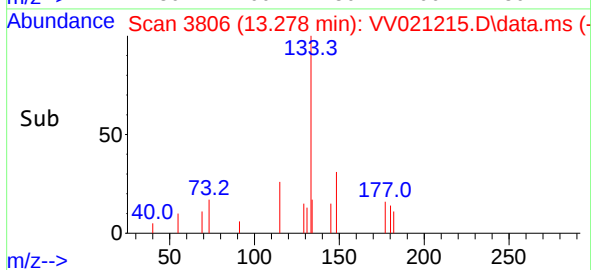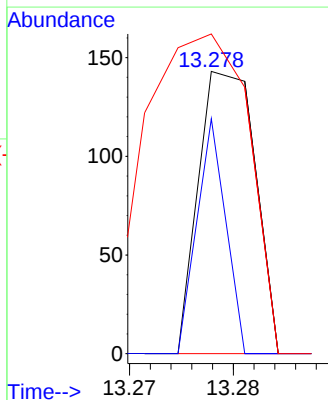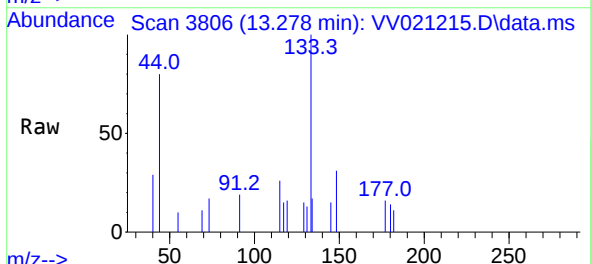

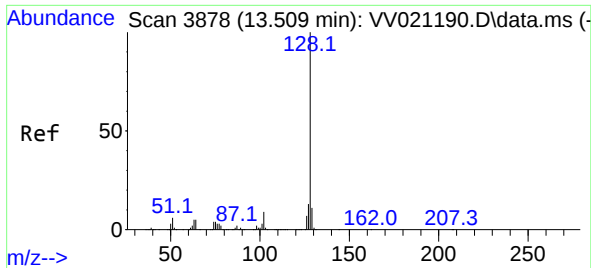

#71
Naphthalene
Concen: 0.89 ug/L
RT: 13.513 min Scan# 3879
Delta R.T. 0.003 min
Lab File: VV021215.D
Acq: 28 Apr 2021 20:55

Instrument :
MSVOA_V
ClientSampleId :
VBLK20

Tgt Ion:	128	Resp:	154
Ion	Ratio	Lower	Upper
128	100		
127	0.0	10.3	15.5#
129	0.0	8.6	13.0#

