

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042821\
 Data File : VV021192.D
 Acq On : 28 Apr 2021 11:34
 Operator : SY/MD
 Sample : VV0428WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK176

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

Signal : TIC: VV021192.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	77	84	100	rBV	431692	436607	14.79%	1.910%
2	1.571	158	165	180	rVB	348498	391938	13.28%	1.714%
3	2.111	323	333	369	rVB	745797	1122250	38.01%	4.908%
4	2.407	421	425	426	rBV2	942	639	0.02%	0.003%
5	2.577	474	478	482	rBV3	950	893	0.03%	0.004%
6	2.706	516	518	520	rBV3	474	223	0.01%	0.001%
7	2.735	524	527	530	rBV	850	744	0.03%	0.003%
8	2.767	533	537	538	rBV4	1628	1147	0.04%	0.005%
9	2.851	561	563	565	rBV	454	236	0.01%	0.001%
10	2.863	565	567	569	rBV2	775	416	0.01%	0.002%
11	2.892	575	576	577	rBV2	237	64	0.00%	0.000%
12	2.902	577	579	581	rBV2	638	306	0.01%	0.001%
13	3.037	618	621	624	rVB	557	258	0.01%	0.001%
14	3.056	624	627	629	rBV2	813	435	0.01%	0.002%
15	3.137	649	652	653	rBV2	398	212	0.01%	0.001%
16	3.191	659	669	671	rBV2	1226	1615	0.05%	0.007%
17	3.355	715	720	721	rBV2	415	314	0.01%	0.001%
18	3.384	727	729	733	rBV2	409	304	0.01%	0.001%
19	3.426	740	742	745	rBV2	443	255	0.01%	0.001%
20	3.471	754	756	764	rVB4	498	491	0.02%	0.002%
21	3.506	764	767	769	rBV2	754	406	0.01%	0.002%
22	3.532	773	775	779	rVB	368	185	0.01%	0.001%
23	3.635	805	807	810	rVB3	602	297	0.01%	0.001%
24	3.706	825	829	833	rVB3	612	546	0.02%	0.002%
25	3.732	833	837	840	rBV3	788	645	0.02%	0.003%
26	3.773	847	850	854	rVB2	628	400	0.01%	0.002%
27	3.799	854	858	860	rBV	566	515	0.02%	0.002%
28	3.867	873	879	880	rBV	661	493	0.02%	0.002%
29	3.908	880	892	941	rVV	145018	554413	18.78%	2.425%
30	4.355	1013	1031	1060	rBV	503168	1243365	42.12%	5.438%
31	4.754	1153	1155	1158	rBV4	731	411	0.01%	0.002%
32	4.776	1158	1162	1166	rVV3	579	597	0.02%	0.003%
33	4.918	1201	1206	1208	rBV2	448	365	0.01%	0.002%
34	4.966	1219	1221	1225	rVB3	894	590	0.02%	0.003%
35	4.995	1225	1230	1231	rBV3	697	634	0.02%	0.003%
36	5.053	1231	1248	1284	rBV3	1139789	2952281	100.00%	12.912%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042821\
 Data File : VV021192.D
 Acq On : 28 Apr 2021 11:34
 Operator : SY/MD
 Sample : VV0428WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK176

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

37	5.497	1384	1386	1387	rBV	721	273	0.01%	0.001%
38	5.622	1413	1425	1452	rBV	863321	1751979	59.34%	7.662%
39	5.915	1505	1516	1535	rBV2	31229	68225	2.31%	0.298%
40	6.014	1545	1547	1548	rBV2	893	404	0.01%	0.002%
41	6.075	1552	1566	1594	rBV	646929	1314950	44.54%	5.751%
42	6.490	1692	1695	1697	rBV2	944	609	0.02%	0.003%
43	6.567	1716	1719	1725	rVB5	1001	957	0.03%	0.004%
44	6.645	1741	1743	1745	rBV2	710	402	0.01%	0.002%
45	6.702	1757	1761	1765	rBV4	1301	1231	0.04%	0.005%
46	6.719	1765	1766	1767	rVV	479	162	0.01%	0.001%
47	6.728	1767	1769	1772	rVB2	973	437	0.01%	0.002%
48	6.751	1772	1776	1777	rBV	440	316	0.01%	0.001%
49	6.764	1777	1780	1784	rBV4	701	585	0.02%	0.003%
50	6.992	1837	1851	1873	rBV2	361098	665305	22.54%	2.910%
51	7.320	1941	1953	1971	rBV	1436801	2468795	83.62%	10.797%
52	7.625	2039	2048	2074	rBV	250589	449083	15.21%	1.964%
53	8.095	2184	2194	2229	rBV	631929	1225548	41.51%	5.360%
54	8.529	2327	2329	2331	rBV3	566	245	0.01%	0.001%
55	8.641	2359	2364	2365	rBV2	765	598	0.02%	0.003%
56	8.857	2419	2431	2461	rBV	1330909	2190568	74.20%	9.581%
57	9.079	2498	2500	2504	rBV2	782	489	0.02%	0.002%
58	9.355	2584	2586	2589	rVB3	1125	637	0.02%	0.003%
59	9.371	2589	2591	2592	rBV	413	169	0.01%	0.001%
60	9.657	2677	2680	2681	rBV	402	230	0.01%	0.001%
61	9.741	2703	2706	2708	rBV3	774	413	0.01%	0.002%
62	9.770	2712	2715	2717	rBV2	548	275	0.01%	0.001%
63	9.783	2717	2719	2720	rBV2	487	191	0.01%	0.001%
64	9.828	2729	2733	2735	rBV2	620	438	0.01%	0.002%
65	9.892	2751	2753	2755	rBV	425	231	0.01%	0.001%
66	10.053	2798	2803	2807	rBV3	653	717	0.02%	0.003%
67	10.130	2821	2827	2835	rVB6	7876	11108	0.38%	0.049%
68	10.223	2843	2856	2877	rBV	944373	1527804	51.75%	6.682%
69	10.471	2927	2933	2937	rBV5	1150	1408	0.05%	0.006%
70	10.548	2952	2957	2959	rBV4	2275	2173	0.07%	0.010%
71	10.718	3008	3010	3012	rBV2	422	177	0.01%	0.001%
72	10.789	3030	3032	3034	rBV3	763	345	0.01%	0.002%
73	10.850	3048	3051	3054	rBV3	923	740	0.03%	0.003%
74	10.924	3065	3074	3084	rBV6	8943	14163	0.48%	0.062%
75	10.998	3095	3097	3100	rBV3	529	264	0.01%	0.001%
76	11.040	3106	3110	3117	rVB5	1402	1730	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042821\
 Data File : VV021192.D
 Acq On : 28 Apr 2021 11:34
 Operator : SY/MD
 Sample : VV0428WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK176

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M

Title : VOC Analysis

77	11.082	3121	3123	3126	rBV	537	463	0.02%	0.002%
78	11.255	3165	3177	3197	rBV	1342680	2089843	70.79%	9.140%
79	11.632	3282	3294	3314	rBV	1486315	2344905	79.43%	10.256%
80	11.963	3394	3397	3400	rBV3	1230	796	0.03%	0.003%
81	12.313	3503	3506	3510	rBV3	805	739	0.03%	0.003%
82	12.654	3608	3612	3624	rVB7	4378	6605	0.22%	0.029%
83	13.374	3832	3836	3837	rBV2	855	621	0.02%	0.003%
84	13.397	3841	3843	3845	rBV2	777	444	0.02%	0.002%
85	14.033	4039	4041	4043	rBV2	902	432	0.01%	0.002%




Sum of corrected areas: 22864712

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042821\
Data File : VV021192.D
Acq On : 28 Apr 2021 11:34
Operator : SY/MD
Sample : VV0428WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK176

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

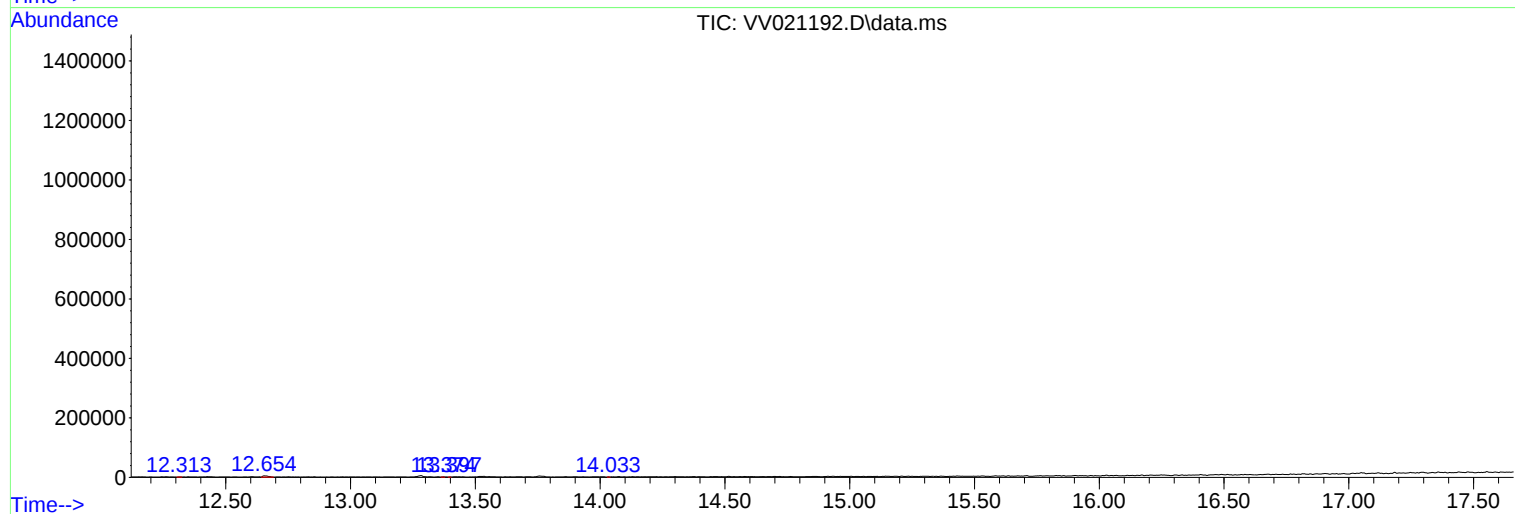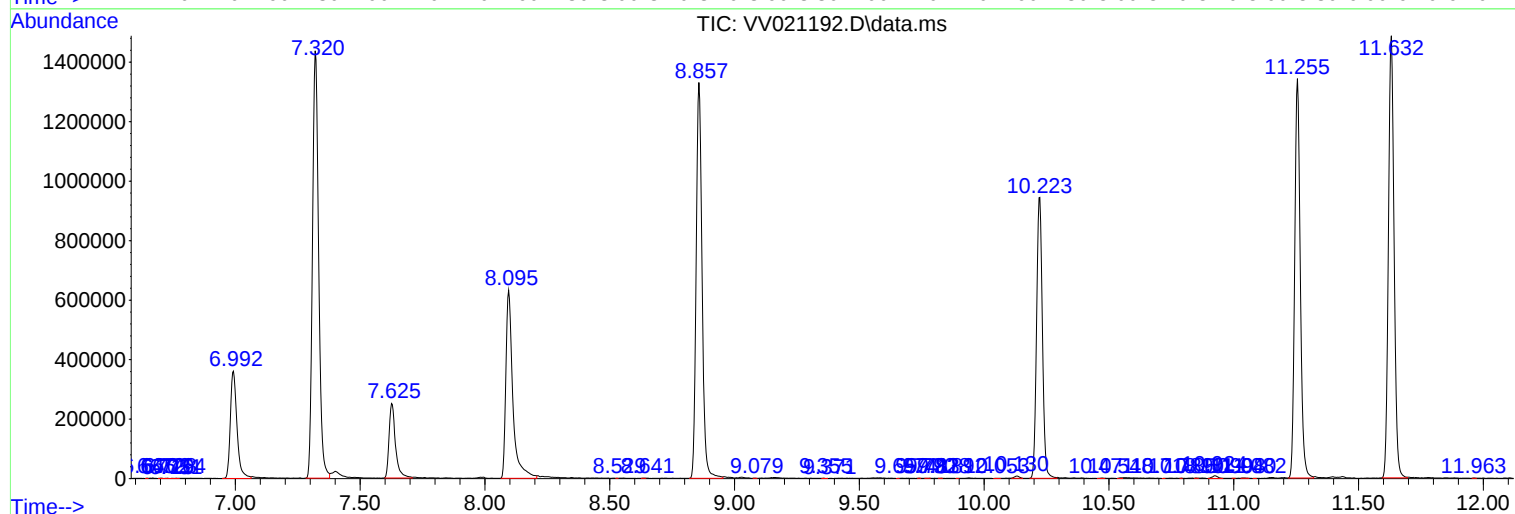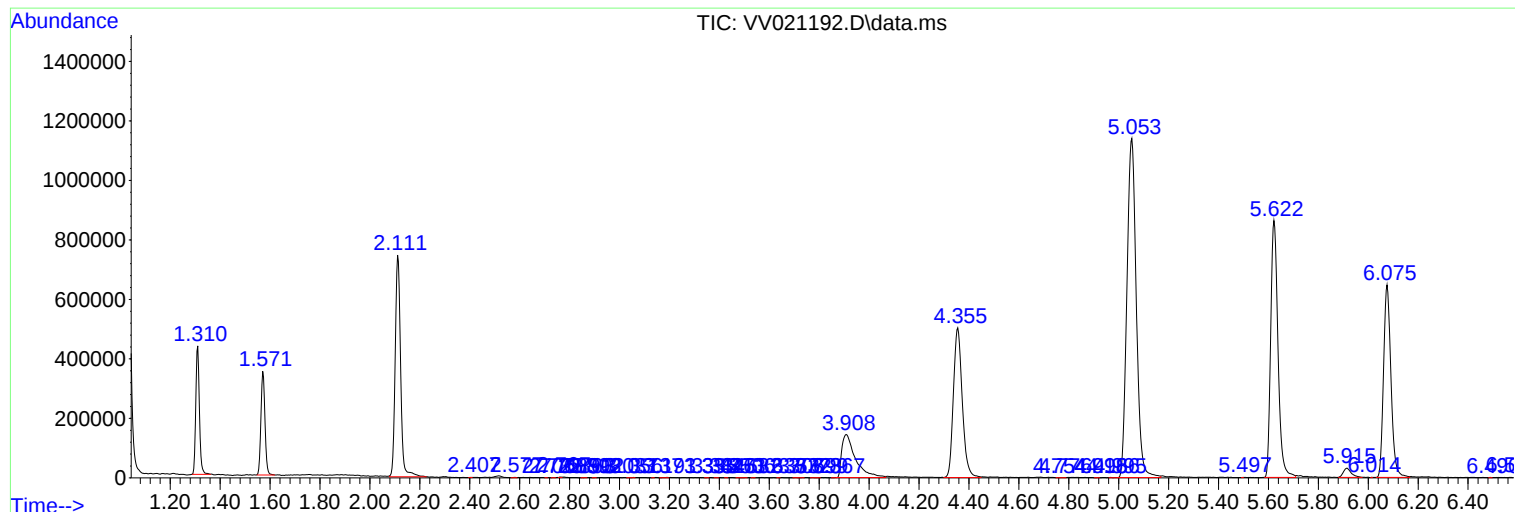

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042821\
Data File : VV021192.D
Acq On : 28 Apr 2021 11:34
Operator : SY/MD
Sample : VV0428WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK176

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042821\
Data File : VV021192.D
Acq On : 28 Apr 2021 11:34
Operator : SY/MD
Sample : VV0428WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK176

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
