

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042821\
 Data File : VV021196.D
 Acq On : 28 Apr 2021 13:07
 Operator : SY/MD
 Sample : VIBLK173
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK173

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M

Title : VOC Analysis

Signal : TIC: VV021196.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	97	rBV	354388	360221	13.37%	1.742%
2	1.571	158	165	177	rVB	305682	339334	12.59%	1.641%
3	2.111	323	333	354	rVB	623901	906333	33.63%	4.383%
4	2.362	408	411	412	rBV2	764	451	0.02%	0.002%
5	2.510	451	457	465	rBV2	7935	11663	0.43%	0.056%
6	2.584	476	480	483	rBV2	905	728	0.03%	0.004%
7	2.629	488	494	499	rBV5	1437	1601	0.06%	0.008%
8	2.761	527	535	538	rBV4	1041	1403	0.05%	0.007%
9	2.793	542	545	548	rVB3	836	541	0.02%	0.003%
10	2.986	602	605	607	rBV2	663	433	0.02%	0.002%
11	3.053	620	626	628	rBV2	895	845	0.03%	0.004%
12	3.114	641	645	647	rVB2	688	348	0.01%	0.002%
13	3.130	647	650	651	rBV	588	362	0.01%	0.002%
14	3.169	659	662	666	rVB3	516	397	0.01%	0.002%
15	3.195	666	670	672	rBV2	848	771	0.03%	0.004%
16	3.259	686	690	692	rVB2	461	342	0.01%	0.002%
17	3.294	697	701	703	rBV2	543	430	0.02%	0.002%
18	3.487	757	761	764	rBV	753	707	0.03%	0.003%
19	3.529	770	774	777	rBV3	762	443	0.02%	0.002%
20	3.548	777	780	784	rBV3	490	498	0.02%	0.002%
21	3.716	829	832	837	rVB3	931	812	0.03%	0.004%
22	3.744	837	841	843	rBV2	513	403	0.01%	0.002%
23	3.802	856	859	863	rVB2	605	399	0.01%	0.002%
24	3.905	878	891	927	rBV2	149617	554735	20.58%	2.683%
25	4.352	1016	1030	1056	rBV	454857	1113152	41.31%	5.383%
26	4.625	1112	1115	1119	rVB3	1352	813	0.03%	0.004%
27	4.941	1209	1213	1219	rVV4	1036	927	0.03%	0.004%
28	5.050	1230	1247	1281	rBV2	1043429	2694863	100.00%	13.032%
29	5.371	1345	1347	1349	rBV2	658	360	0.01%	0.002%
30	5.394	1351	1354	1356	rVV4	1106	709	0.03%	0.003%
31	5.423	1360	1363	1366	rVB4	1186	826	0.03%	0.004%
32	5.484	1380	1382	1385	rBV3	652	344	0.01%	0.002%
33	5.545	1399	1401	1405	rBV2	605	433	0.02%	0.002%
34	5.568	1405	1408	1409	rBV2	880	417	0.02%	0.002%
35	5.622	1413	1425	1451	rBV	751787	1520684	56.43%	7.354%
36	5.912	1506	1515	1530	rBV3	33464	70334	2.61%	0.340%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042821\
 Data File : VW021196.D
 Acq On : 28 Apr 2021 13:07
 Operator : SY/MD
 Sample : VIBLK173
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK173

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

37	6.076	1551	1566	1590	rBV	584245	1204323	44.69%	5.824%
38	6.352	1649	1652	1655	rBV3	1175	933	0.03%	0.005%
39	6.410	1668	1670	1672	rBV2	854	513	0.02%	0.002%
40	6.432	1675	1677	1680	rVB2	1036	470	0.02%	0.002%
41	6.516	1701	1703	1705	rBV2	729	368	0.01%	0.002%
42	6.545	1708	1712	1717	rVV4	1212	1150	0.04%	0.006%
43	6.789	1783	1788	1790	rBV3	552	447	0.02%	0.002%
44	6.825	1795	1799	1800	rBV3	520	384	0.01%	0.002%
45	6.889	1815	1819	1821	rBV2	713	432	0.02%	0.002%
46	6.989	1839	1850	1875	rBV	327775	609201	22.61%	2.946%
47	7.246	1927	1930	1931	rBV2	1867	1089	0.04%	0.005%
48	7.320	1941	1953	1973	rBV	1235579	2141049	79.45%	10.353%
49	7.625	2038	2048	2068	rBV	237910	416583	15.46%	2.014%
50	7.805	2102	2104	2106	rBV2	1099	544	0.02%	0.003%
51	7.982	2148	2159	2173	rVV3	90756	158690	5.89%	0.767%
52	8.095	2184	2194	2225	rBV	629446	1207372	44.80%	5.838%
53	8.500	2317	2320	2326	rBV3	1332	1295	0.05%	0.006%
54	8.526	2326	2328	2331	rBV2	777	549	0.02%	0.003%
55	8.603	2349	2352	2353	rBV	659	413	0.02%	0.002%
56	8.764	2398	2402	2406	rBV3	767	574	0.02%	0.003%
57	8.786	2406	2409	2411	rBV2	723	460	0.02%	0.002%
58	8.857	2419	2431	2456	rBV	1177422	1924615	71.42%	9.307%
59	9.281	2559	2563	2564	rBV2	716	444	0.02%	0.002%
60	9.352	2582	2585	2590	rBV3	401	398	0.01%	0.002%
61	9.381	2590	2594	2598	rVB2	1033	866	0.03%	0.004%
62	9.419	2601	2606	2608	rBV2	639	680	0.03%	0.003%
63	9.432	2608	2610	2615	rVB	938	695	0.03%	0.003%
64	9.487	2624	2627	2629	rVB2	883	493	0.02%	0.002%
65	9.510	2631	2634	2636	rBV2	722	453	0.02%	0.002%
66	9.529	2636	2640	2644	rBV3	782	874	0.03%	0.004%
67	9.600	2660	2662	2665	rBV	676	443	0.02%	0.002%
68	9.719	2697	2699	2704	rBV4	927	758	0.03%	0.004%
69	9.783	2717	2719	2727	rVB4	821	811	0.03%	0.004%
70	9.850	2737	2740	2744	rBV2	1034	729	0.03%	0.004%
71	9.921	2759	2762	2764	rBV3	757	420	0.02%	0.002%
72	9.995	2783	2785	2792	rVB5	899	725	0.03%	0.004%
73	10.059	2803	2805	2807	rVB2	1079	452	0.02%	0.002%
74	10.133	2820	2828	2839	rVB6	6037	9817	0.36%	0.047%
75	10.220	2844	2855	2880	rBV	908254	1461320	54.23%	7.067%
76	10.554	2951	2959	2963	rBV5	2035	2838	0.11%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042821\
 Data File : VV021196.D
 Acq On : 28 Apr 2021 13:07
 Operator : SY/MD
 Sample : VIBLK173
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK173

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

77	10.731	3011	3014	3018	rBV	630	421	0.02%	0.002%
78	10.789	3028	3032	3034	rBV3	683	459	0.02%	0.002%
79	10.860	3051	3054	3059	rBV5	946	768	0.03%	0.004%
80	10.924	3066	3074	3086	rVB5	6390	9792	0.36%	0.047%
81	10.989	3091	3094	3096	rBV	723	526	0.02%	0.003%
82	11.037	3104	3109	3111	rBV3	1334	1051	0.04%	0.005%
83	11.108	3129	3131	3134	rBV2	538	362	0.01%	0.002%
84	11.156	3136	3146	3151	rVV2	3216	4590	0.17%	0.022%
85	11.255	3165	3177	3203	rBV	1183554	1832384	68.00%	8.861%
86	11.477	3244	3246	3248	rBV2	1243	679	0.03%	0.003%
87	11.535	3260	3264	3266	rBV3	954	839	0.03%	0.004%
88	11.632	3281	3294	3315	rBV	1311876	2074144	76.97%	10.030%
89	11.850	3355	3362	3364	rBV5	1637	1998	0.07%	0.010%
90	11.898	3374	3377	3378	rBV2	893	579	0.02%	0.003%
91	12.027	3415	3417	3420	rBV3	848	438	0.02%	0.002%
92	12.169	3459	3461	3465	rVB2	1252	714	0.03%	0.003%
93	12.191	3465	3468	3470	rBV3	915	604	0.02%	0.003%
94	12.410	3532	3536	3543	rBV3	1091	1242	0.05%	0.006%
95	12.448	3543	3548	3551	rBV4	1202	1064	0.04%	0.005%
96	12.657	3609	3613	3620	rBV6	1924	2408	0.09%	0.012%
97	12.847	3669	3672	3673	rBV3	899	446	0.02%	0.002%
98	13.230	3789	3791	3793	rBV	1122	583	0.02%	0.003%
99	13.329	3820	3822	3824	rBV2	783	350	0.01%	0.002%
100	13.390	3839	3841	3843	rBV	674	363	0.01%	0.002%




Sum of corrected areas: 20679536

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042821\
Data File : VV021196.D
Acq On : 28 Apr 2021 13:07
Operator : SY/MD
Sample : VIBLK173
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK173

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

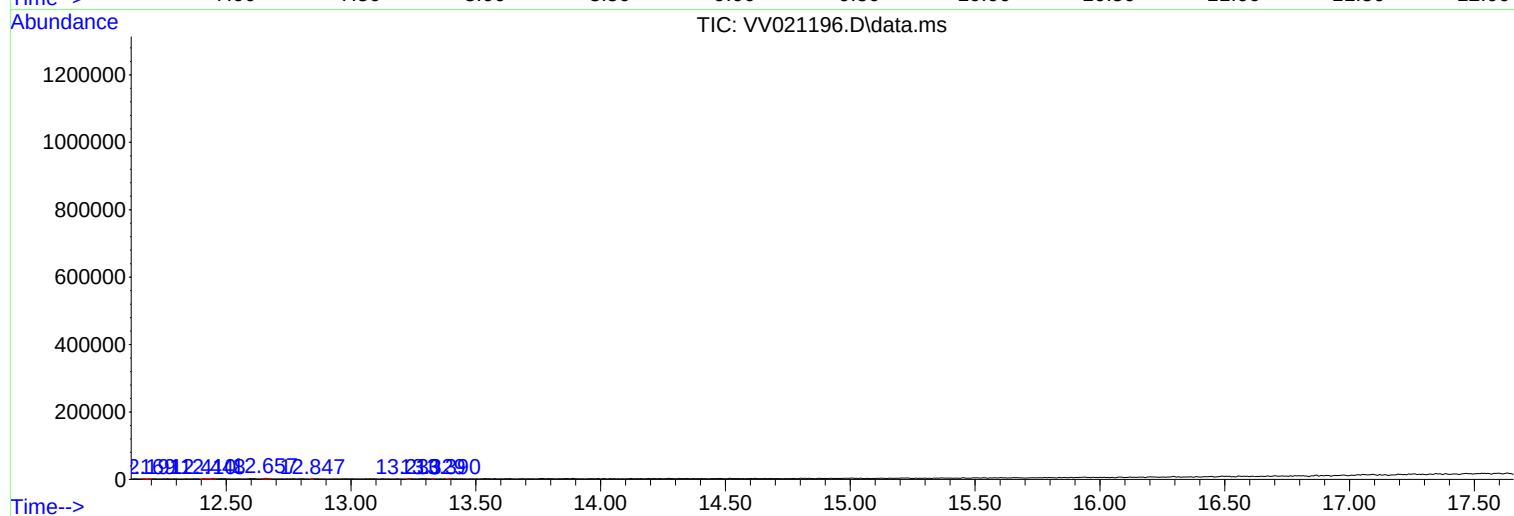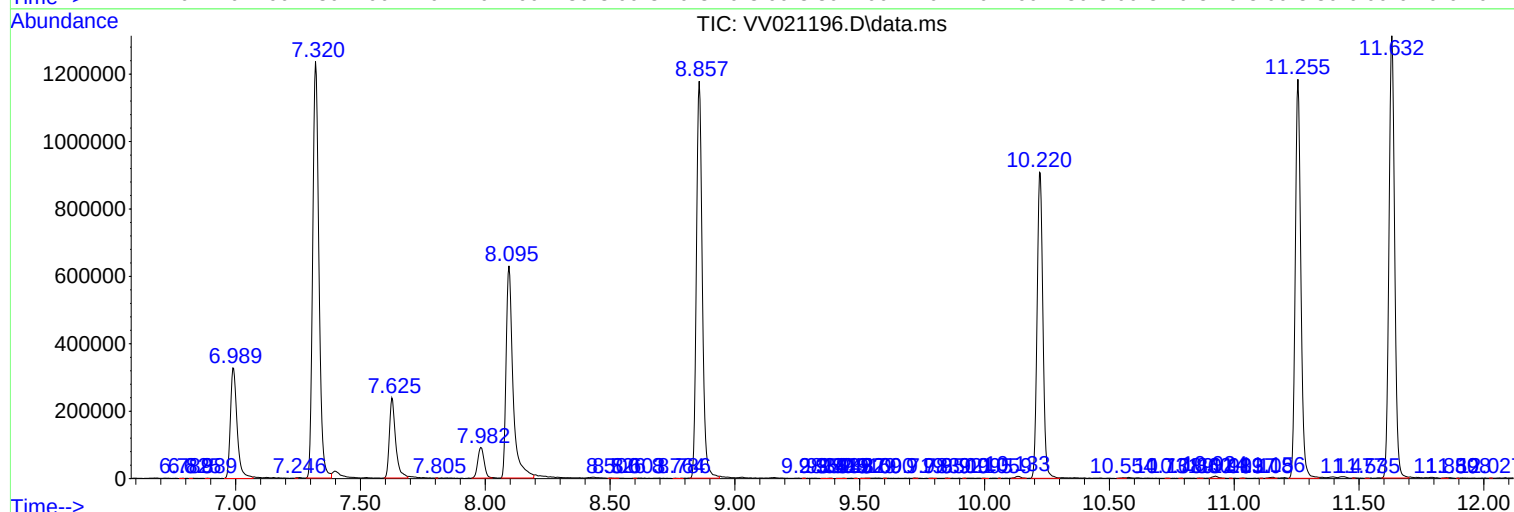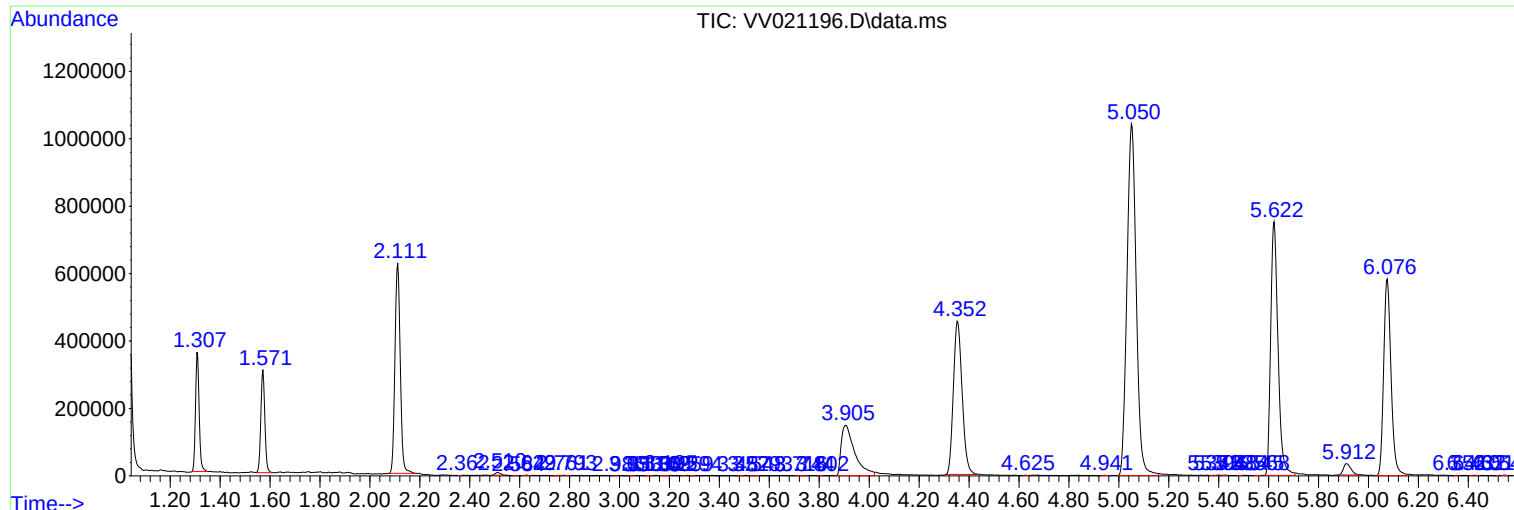

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042821\
Data File : VV021196.D
Acq On : 28 Apr 2021 13:07
Operator : SY/MD
Sample : VIBLK173
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK173

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042821\
Data File : VV021196.D
Acq On : 28 Apr 2021 13:07
Operator : SY/MD
Sample : VIBLK173
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK173

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
