

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042821\
 Data File : VV021208.D
 Acq On : 28 Apr 2021 17:48
 Operator : SY/MD
 Sample : M2181-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M

Title : VOC Analysis

Signal : TIC: VV021208.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	97	rVB	376739	371784	13.92%	1.771%
2	1.571	158	165	179	rVB	309561	350753	13.13%	1.670%
3	2.111	323	333	366	rVB	654445	982476	36.78%	4.679%
4	2.362	408	411	414	rBV3	677	634	0.02%	0.003%
5	2.433	431	433	436	rBV3	906	475	0.02%	0.002%
6	2.513	449	458	472	rVB7	5247	10309	0.39%	0.049%
7	2.603	484	486	489	rVB2	621	244	0.01%	0.001%
8	2.632	492	495	498	rVB3	864	494	0.02%	0.002%
9	2.687	509	512	515	rBV2	770	648	0.02%	0.003%
10	2.796	545	546	549	rBV2	359	219	0.01%	0.001%
11	2.841	558	560	564	rVB3	1163	589	0.02%	0.003%
12	2.860	564	566	569	rBV	488	264	0.01%	0.001%
13	2.889	572	575	578	rBV3	741	507	0.02%	0.002%
14	3.021	613	616	622	rBV2	697	688	0.03%	0.003%
15	3.092	636	638	640	rBV3	591	224	0.01%	0.001%
16	3.156	656	658	660	rBV	554	278	0.01%	0.001%
17	3.207	672	674	678	rVB	565	272	0.01%	0.001%
18	3.230	678	681	684	rBV	560	476	0.02%	0.002%
19	3.352	718	719	722	rVB	567	265	0.01%	0.001%
20	3.371	722	725	726	rBV2	542	232	0.01%	0.001%
21	3.407	732	736	739	rVB4	597	485	0.02%	0.002%
22	3.423	739	741	745	rBV2	596	362	0.01%	0.002%
23	3.442	745	747	752	rVB2	549	353	0.01%	0.002%
24	3.474	755	757	759	rVB2	711	235	0.01%	0.001%
25	3.497	761	764	766	rBV2	716	446	0.02%	0.002%
26	3.510	766	768	771	rVB2	975	483	0.02%	0.002%
27	3.529	771	774	777	rBV	809	505	0.02%	0.002%
28	3.568	784	786	789	rBV2	387	212	0.01%	0.001%
29	3.632	802	806	811	rVB3	806	948	0.04%	0.005%
30	3.658	811	814	817	rBV2	556	415	0.02%	0.002%
31	3.674	817	819	824	rBV2	507	408	0.02%	0.002%
32	3.770	845	849	854	rBV2	494	388	0.01%	0.002%
33	3.796	854	857	860	rVB2	391	199	0.01%	0.001%
34	3.815	860	863	864	rBV2	342	184	0.01%	0.001%
35	3.850	872	874	877	rVB3	601	301	0.01%	0.001%
36	3.902	878	890	933	rBV	146695	538915	20.18%	2.567%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042821\
 Data File : VV021208.D
 Acq On : 28 Apr 2021 17:48
 Operator : SY/MD
 Sample : M2181-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

37	4.352	1015	1030	1058	rBV	447439	1109077	41.52%	5.282%
38	4.889	1193	1197	1200	rBV4	955	859	0.03%	0.004%
39	5.050	1229	1247	1285	rBV2	1035805	2671113	100.00%	12.721%
40	5.420	1360	1362	1364	rBV3	758	336	0.01%	0.002%
41	5.436	1364	1367	1370	rVB3	981	520	0.02%	0.002%
42	5.500	1385	1387	1389	rBV	1246	614	0.02%	0.003%
43	5.558	1402	1405	1408	rBV2	899	626	0.02%	0.003%
44	5.622	1412	1425	1450	rBV	823589	1649977	61.77%	7.858%
45	5.911	1506	1515	1533	rVB2	36976	73076	2.74%	0.348%
46	6.075	1548	1566	1590	rBV	588532	1203009	45.04%	5.729%
47	6.284	1629	1631	1633	rBV3	1083	508	0.02%	0.002%
48	6.420	1672	1673	1675	rBV2	507	197	0.01%	0.001%
49	6.439	1677	1679	1684	rVB2	1091	701	0.03%	0.003%
50	6.461	1684	1686	1688	rBV	559	364	0.01%	0.002%
51	6.493	1694	1696	1701	rVB3	889	706	0.03%	0.003%
52	6.526	1704	1706	1709	rBV2	462	343	0.01%	0.002%
53	6.551	1710	1714	1717	rVV5	811	638	0.02%	0.003%
54	6.612	1731	1733	1736	rVV2	570	293	0.01%	0.001%
55	6.674	1751	1752	1757	rVB2	1170	709	0.03%	0.003%
56	6.712	1757	1764	1767	rBV5	998	1390	0.05%	0.007%
57	6.773	1781	1783	1786	rVB3	1046	490	0.02%	0.002%
58	6.825	1795	1799	1800	rBV2	609	388	0.01%	0.002%
59	6.860	1807	1810	1813	rBV	859	455	0.02%	0.002%
60	6.905	1821	1824	1827	rBV	496	360	0.01%	0.002%
61	6.950	1833	1838	1839	rBV	735	606	0.02%	0.003%
62	6.989	1839	1850	1876	rBV	314582	582748	21.82%	2.775%
63	7.320	1939	1953	1972	rBV	1265448	2189868	81.98%	10.429%
64	7.625	2037	2048	2069	rBV	227346	402494	15.07%	1.917%
65	7.870	2123	2124	2130	rVB6	1184	911	0.03%	0.004%
66	7.982	2152	2159	2171	rVB6	12285	21233	0.79%	0.101%
67	8.095	2184	2194	2228	rBV	624166	1207798	45.22%	5.752%
68	8.554	2335	2337	2338	rBV2	689	337	0.01%	0.002%
69	8.680	2371	2376	2378	rBV2	1221	1063	0.04%	0.005%
70	8.808	2414	2416	2417	rBV2	627	247	0.01%	0.001%
71	8.857	2420	2431	2453	rBV	1267261	2051406	76.80%	9.770%
72	9.120	2511	2513	2518	rBV4	898	698	0.03%	0.003%
73	9.207	2537	2540	2545	rBV4	1066	1243	0.05%	0.006%
74	9.349	2582	2584	2587	rBV2	776	579	0.02%	0.003%
75	9.484	2620	2626	2627	rBV5	749	675	0.03%	0.003%
76	9.506	2631	2633	2636	rVV2	616	274	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042821\
 Data File : VV021208.D
 Acq On : 28 Apr 2021 17:48
 Operator : SY/MD
 Sample : M2181-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

77	9.596	2657	2661	2663	rBV2	779	576	0.02%	0.003%
78	9.683	2684	2688	2691	rBV4	1062	981	0.04%	0.005%
79	9.786	2718	2720	2723	rVB	705	299	0.01%	0.001%
80	9.908	2754	2758	2759	rBV2	855	592	0.02%	0.003%
81	10.095	2814	2816	2820	rVB	551	332	0.01%	0.002%
82	10.133	2820	2828	2839	rBV5	5975	9589	0.36%	0.046%
83	10.172	2839	2840	2842	rBV	519	235	0.01%	0.001%
84	10.220	2844	2855	2877	rVV	881468	1399356	52.39%	6.664%
85	10.416	2914	2916	2920	rBV2	815	493	0.02%	0.002%
86	10.448	2924	2926	2927	rBV2	796	313	0.01%	0.001%
87	10.532	2947	2952	2955	rBV3	741	881	0.03%	0.004%
88	10.728	3009	3013	3014	rBV2	485	336	0.01%	0.002%
89	10.988	3093	3094	3096	rBV	415	193	0.01%	0.001%
90	11.152	3139	3145	3152	rBV4	3002	4218	0.16%	0.020%
91	11.255	3165	3177	3194	rBV	1285719	1987198	74.40%	9.464%
92	11.632	3281	3294	3316	rBV	1356280	2142771	80.22%	10.205%
93	12.066	3427	3429	3431	rBV2	810	337	0.01%	0.002%
94	12.278	3493	3495	3497	rVB2	567	245	0.01%	0.001%
95	12.615	3598	3600	3603	rVB3	1159	544	0.02%	0.003%
96	12.776	3648	3650	3652	rBV	632	303	0.01%	0.001%
97	13.204	3781	3783	3785	rVB	882	338	0.01%	0.002%
98	13.287	3806	3809	3811	rBV2	1273	806	0.03%	0.004%
99	13.387	3838	3840	3842	rVB	796	333	0.01%	0.002%
100	13.403	3842	3845	3848	rBV2	1236	893	0.03%	0.004%


Sum of corrected areas: 20997761

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042821\
Data File : VV021208.D
Acq On : 28 Apr 2021 17:48
Operator : SY/MD
Sample : M2181-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

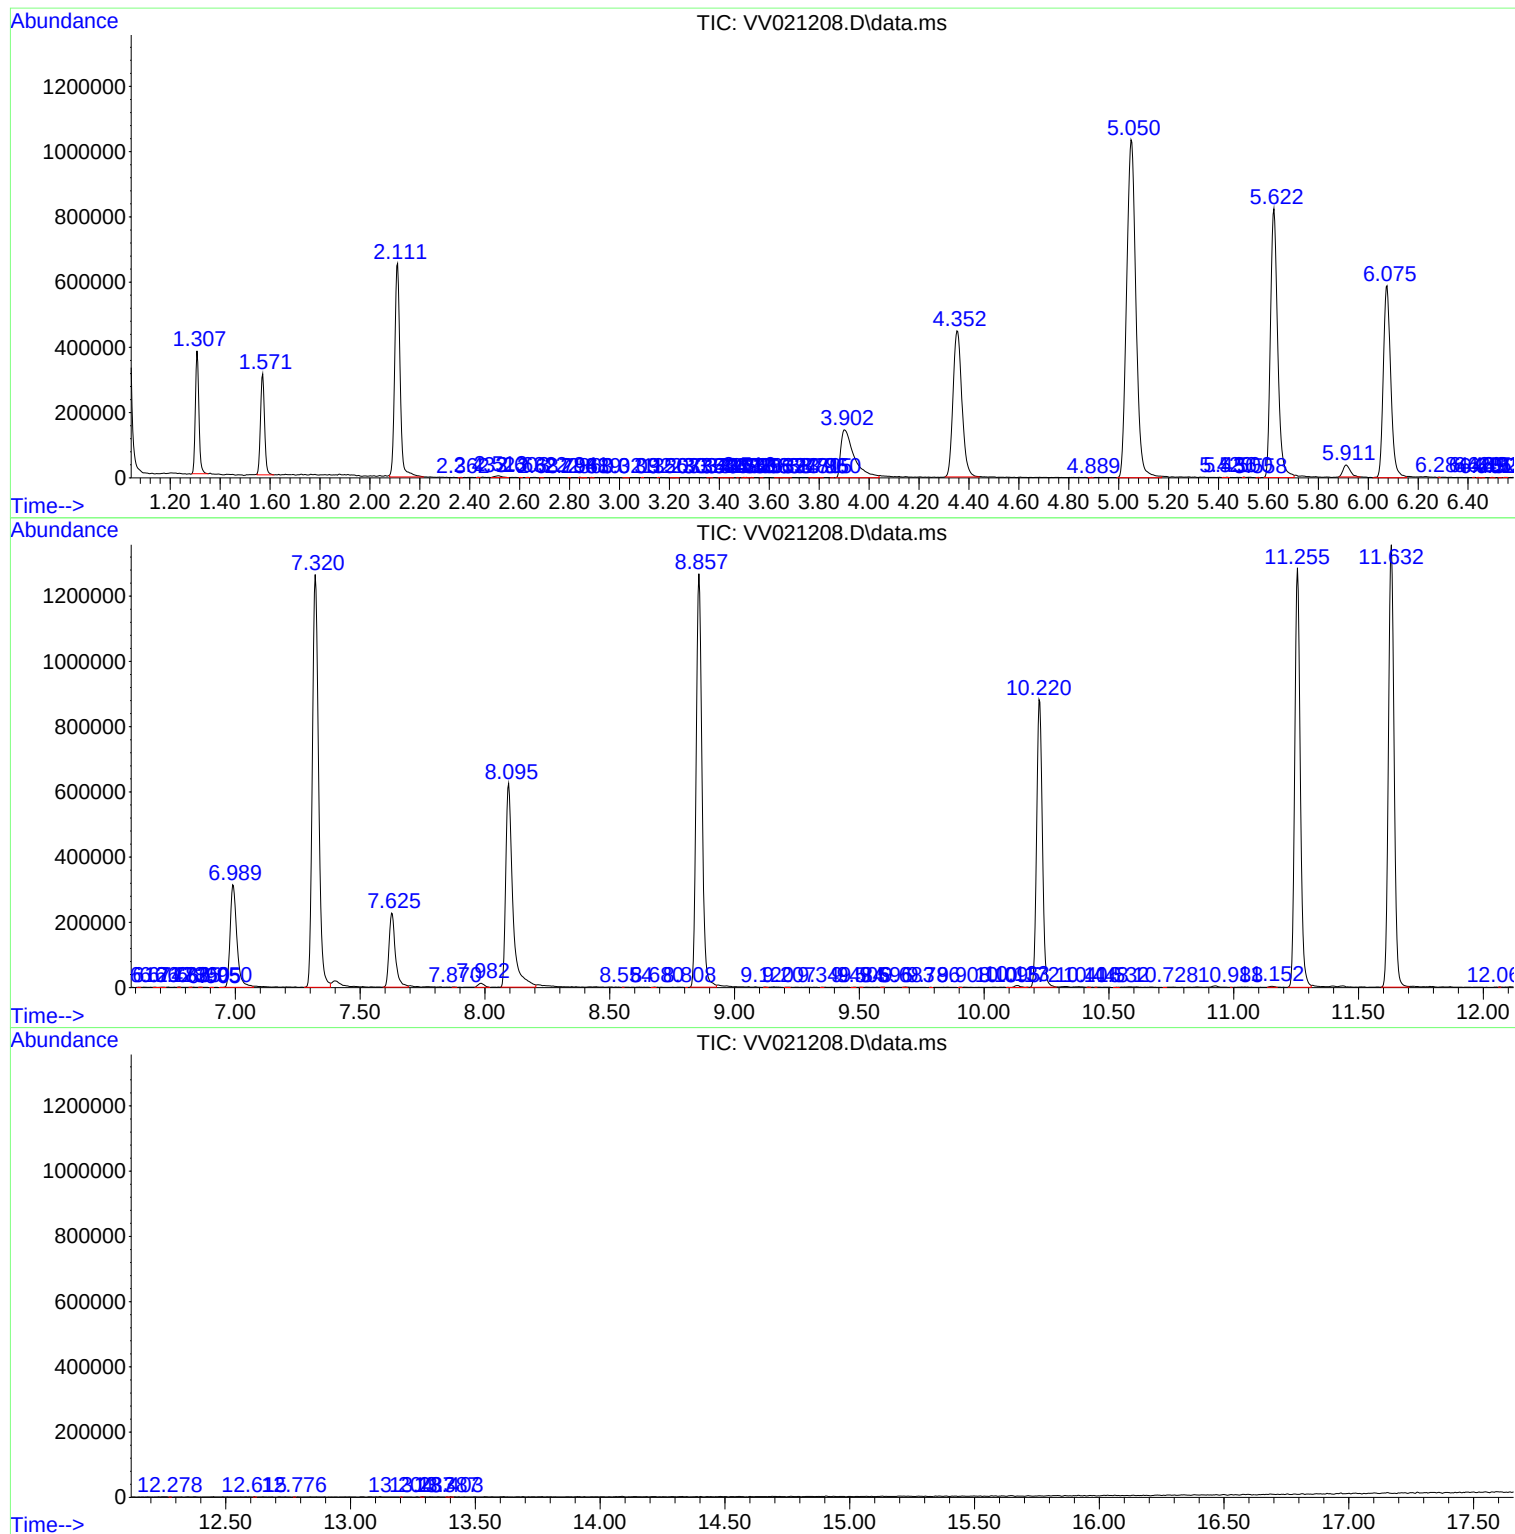

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042821\
Data File : VV021208.D
Acq On : 28 Apr 2021 17:48
Operator : SY/MD
Sample : M2181-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042821\
Data File : VV021208.D
Acq On : 28 Apr 2021 17:48
Operator : SY/MD
Sample : M2181-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc