
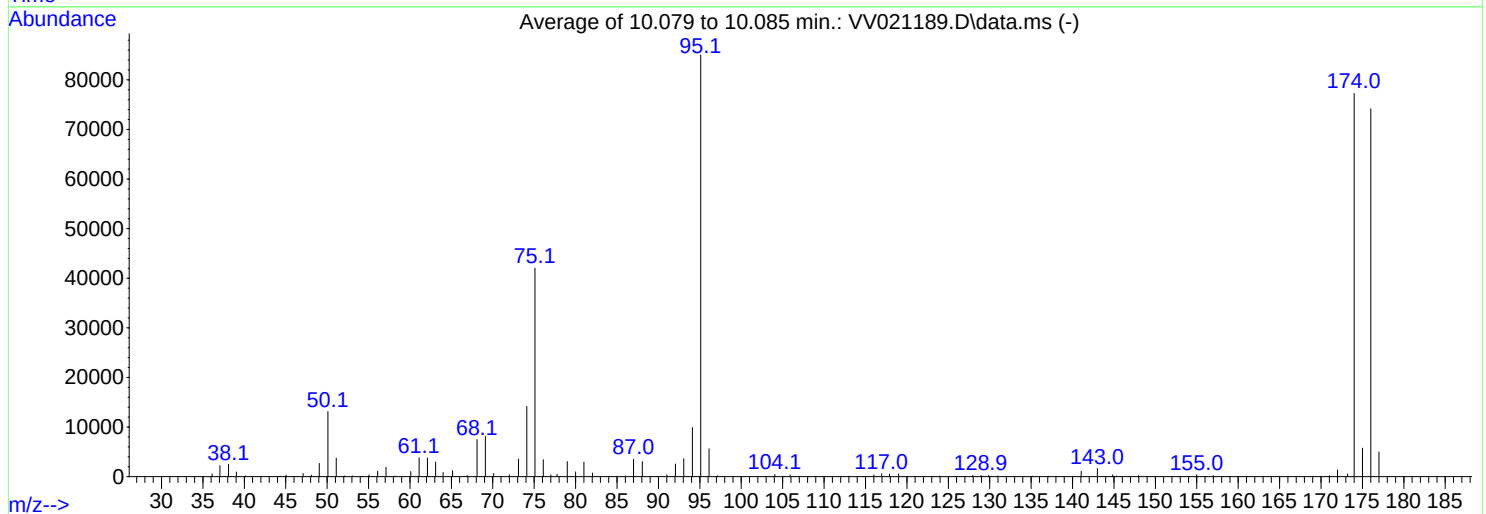


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042821\
 Data File : VV021189.D
 Acq On : 28 Apr 2021 10:03
 Operator : SY/MD
 Sample : BFB91
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB191

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis
 Last Update : Fri Apr 30 05:55:34 2021

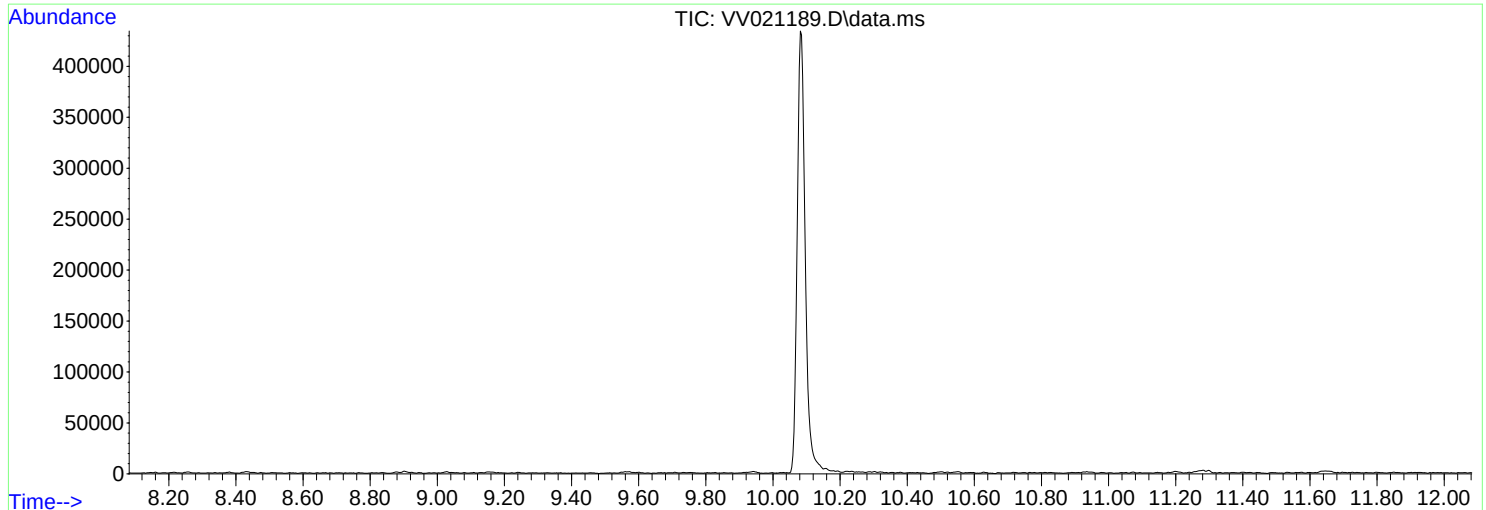

AutoFind: Scans 2811, 2812, 2813; Background Corrected with Scan 2800

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.4	13126	PASS
75	95	30	80	49.4	42045	PASS
95	95	100	100	100.0	85029	PASS
96	95	5	9	6.6	5621	PASS
173	174	0.00	2	0.7	529	PASS
174	95	50	120	90.9	77259	PASS
175	174	5	9	7.4	5734	PASS
176	174	95	105	96.0	74171	PASS
177	176	5	10	6.7	4992	PASS

m/z	Abundance
36.10	577.0
37.10	2205.0
38.10	2502.0
39.00	881.0
40.10	235.0
44.10	792.0
45.00	290.0
47.10	663.0
48.10	285.0
49.10	2736.0
50.10	13644.0
51.10	3851.0
52.20	149.0
53.10	185.0
54.30	130.0
55.00	394.0
56.10	1179.0
57.10	1931.0
58.20	154.0
60.10	1137.0
61.10	3887.0
62.10	3978.0
63.10	3025.0
64.00	901.0
65.10	1281.0
66.90	231.0
68.10	7774.0
69.10	8502.0
70.10	665.0
72.00	385.0
73.10	3669.0
74.10	14538.0
75.10	43904.0
76.10	3403.0
77.00	367.0
77.70	474.0
79.00	3156.0
80.00	978.0
81.00	3002.0
82.00	774.0
86.00	173.0
87.00	3701.0
88.10	3092.0
91.00	430.0
92.10	2618.0
93.10	3666.0
94.10	10117.0
95.10	87856.0
96.10	5797.0
97.20	232.0
104.00	479.0
105.00	125.0
105.90	341.0
113.00	129.0
114.80	103.0
116.00	331.0
116.90	581.0
117.90	524.0
119.00	561.0
123.90	172.0
128.00	258.0
129.00	304.0
129.90	214.0
130.90	202.0
135.20	142.0
137.10	127.0
141.10	1123.0
143.00	1760.0
144.00	120.0
144.80	383.0
145.30	237.0
148.00	241.0
152.90	101.0
155.00	387.0
157.00	249.0
171.00	238.0
172.00	1325.0
174.00	79488.0
175.00	5873.0
176.00	76776.0
177.00	5291.0

Instrument :
MSVOA_V
ClientSampleId :
BFB191

m/z	Abundance
36.10	594.0
37.00	2110.0
38.10	2466.0
39.00	891.0
39.90	269.0
44.10	861.0
45.10	231.0
47.10	638.0
48.00	304.0
49.00	2713.0
50.10	12466.0
51.10	3696.0
52.20	210.0
53.00	192.0
55.10	342.0
56.10	1001.0
57.10	1890.0
58.10	113.0
60.10	906.0
61.10	3764.0
62.10	3514.0
63.10	2680.0
64.00	667.0
65.20	875.0
66.90	289.0
68.10	7150.0
69.10	7588.0
70.10	631.0
72.00	259.0
73.10	3385.0
74.10	14100.0
75.10	40264.0
76.10	3525.0
77.00	412.0
77.90	421.0
79.00	2951.0
80.00	889.0
81.00	2946.0
82.10	669.0
86.00	149.0
87.00	3625.0
88.00	3151.0
91.00	306.0
92.10	2682.0
93.00	3413.0
94.10	8955.0
95.10	80784.0
96.10	5468.0
97.20	236.0
104.10	356.0
106.00	306.0
107.00	125.0
113.00	163.0
116.10	354.0
116.90	482.0
117.90	516.0
118.90	515.0
127.90	251.0
128.90	213.0
129.80	185.0
130.90	189.0
141.00	1199.0
143.00	1727.0
144.00	101.0
144.90	389.0
147.90	201.0
154.10	110.0
155.00	529.0
156.20	105.0
157.00	233.0
161.20	113.0
171.00	223.0
172.00	1283.0
174.00	71296.0
175.00	5522.0
176.00	69320.0
177.00	4641.0

Instrument :
MSVOA_V
ClientSampleId :
BFB191

m/z	Abundance
40.00	214.0
44.10	757.0
49.60	128.0

Instrument :
MSVOA_V
ClientSampleId :
BFB191

m/z	Abundance
36.10	475.0
37.10	2325.0
38.10	2465.0
39.10	1041.0
40.20	225.0
44.20	707.0
45.00	432.0
47.10	639.0
48.20	327.0
49.10	2580.0
50.10	13269.0
51.10	3642.0
52.00	136.0
53.10	143.0
54.30	110.0
55.00	354.0
56.10	1132.0
57.10	1794.0
58.30	173.0
60.10	1096.0
61.10	3788.0
62.10	3798.0
63.10	3134.0
64.00	965.0
65.10	1549.0
67.00	142.0
68.10	7542.0
69.10	8281.0
70.10	600.0
72.00	464.0
73.10	3554.0
74.10	13861.0
75.10	41968.0
76.10	3335.0
77.00	310.0
77.60	533.0
79.00	3020.0
80.00	1014.0
81.00	2898.0
82.00	813.0
86.00	175.0
87.00	3160.0
88.10	2879.0
91.00	475.0
92.00	2352.0
93.10	3763.0
94.10	10643.0
95.10	86448.0
96.10	5599.0
97.10	165.0
102.90	119.0
104.00	558.0
105.00	136.0
105.80	398.0
108.10	144.0
115.90	375.0
117.00	695.0
117.90	481.0
119.10	574.0
123.90	185.0
128.00	236.0
129.00	289.0
129.90	304.0
130.90	136.0
135.20	165.0
137.10	154.0
141.10	981.0
143.00	1476.0
144.80	399.0
145.30	247.0
148.00	201.0
155.00	212.0
157.00	234.0
158.80	114.0
161.00	120.0
171.00	173.0
172.00	1449.0
173.20	1587.0
174.00	80992.0
175.00	5807.0
176.00	76416.0
177.00	5044.0
178.20	122.0

Instrument :
MSVOA_V
ClientSampleId :
BFB191