




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042823\
 Data File : VV030933.D
 Acq On : 28 Apr 2023 20:11
 Operator : SY/MD
 Sample : 02488-19
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHE74

Manual IntegrationsAPPROVED

Quant Time: Apr 29 01:13:24 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Apr 29 01:06:38 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/01/2023
 Supervised By :Mahesh Dadoda 05/01/2023

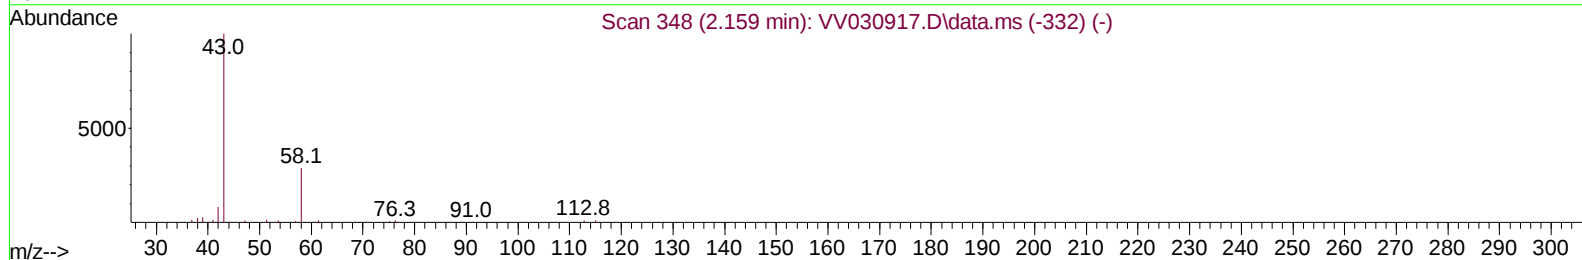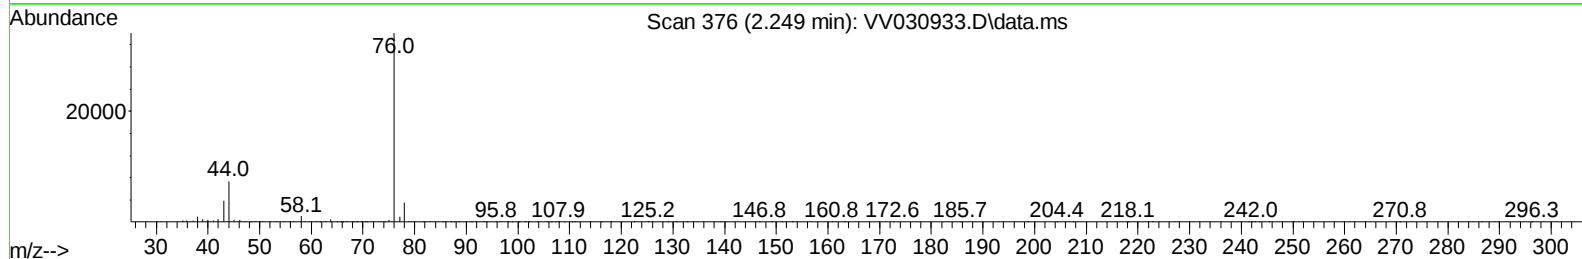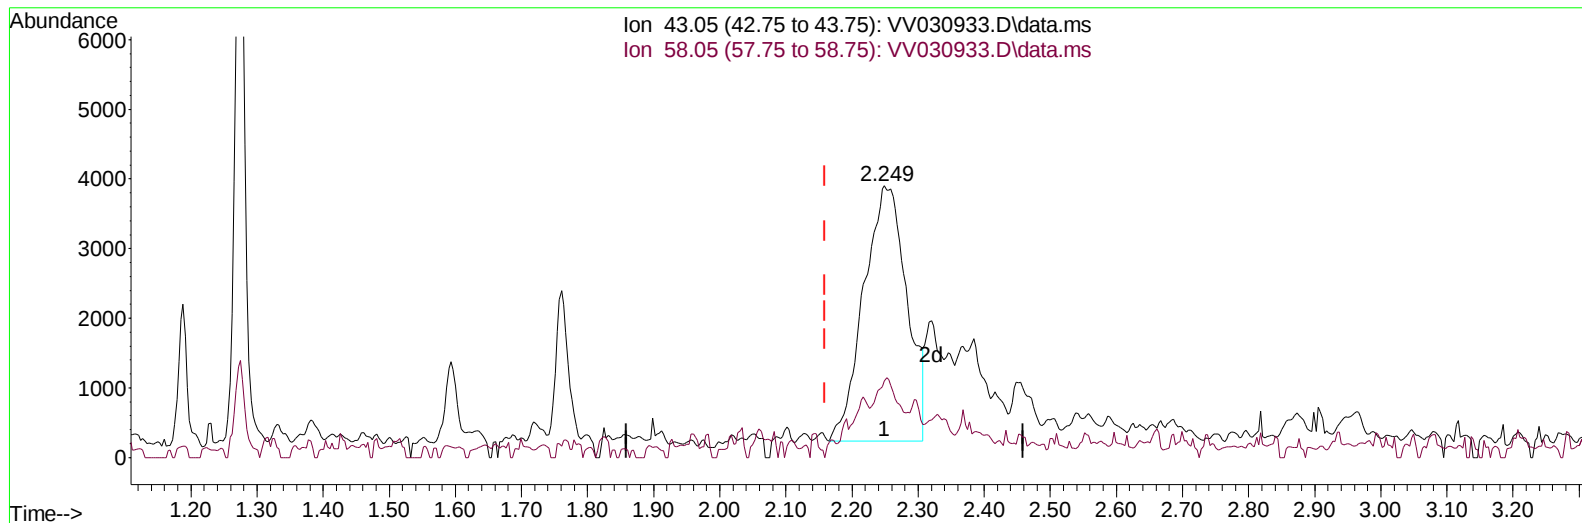

TIC: VV030933.D\data.ms

(13) Acetone (T)

2.249min (+ 0.090) 10.93 ug/L

response 16597

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	18.50	12.23
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042823\
 Data File : VV030933.D
 Acq On : 28 Apr 2023 20:11
 Operator : SY/MD
 Sample : 02488-19
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHE74

Manual IntegrationsAPPROVED

Quant Time: Apr 29 01:13:24 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Apr 29 01:06:38 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/01/2023
 Supervised By :Mahesh Dadoda 05/01/2023

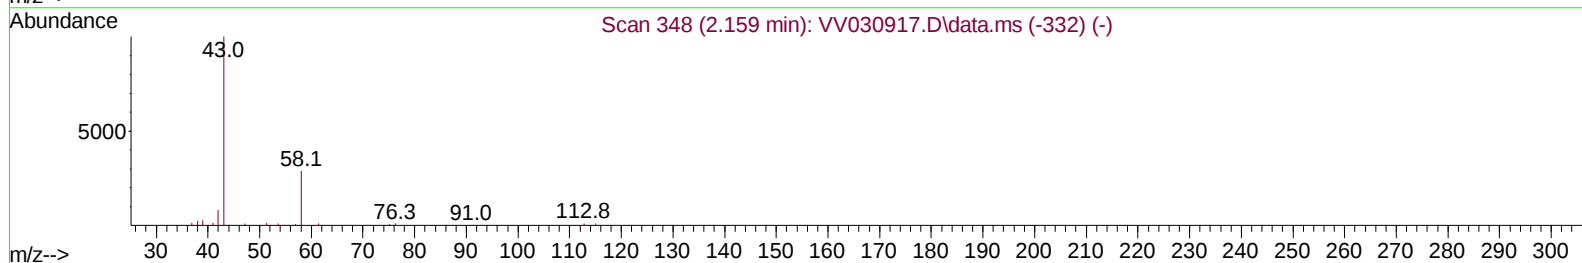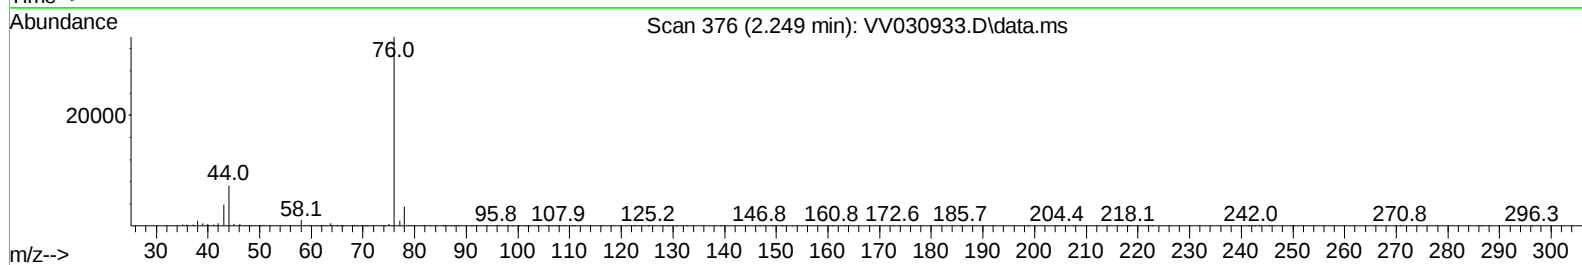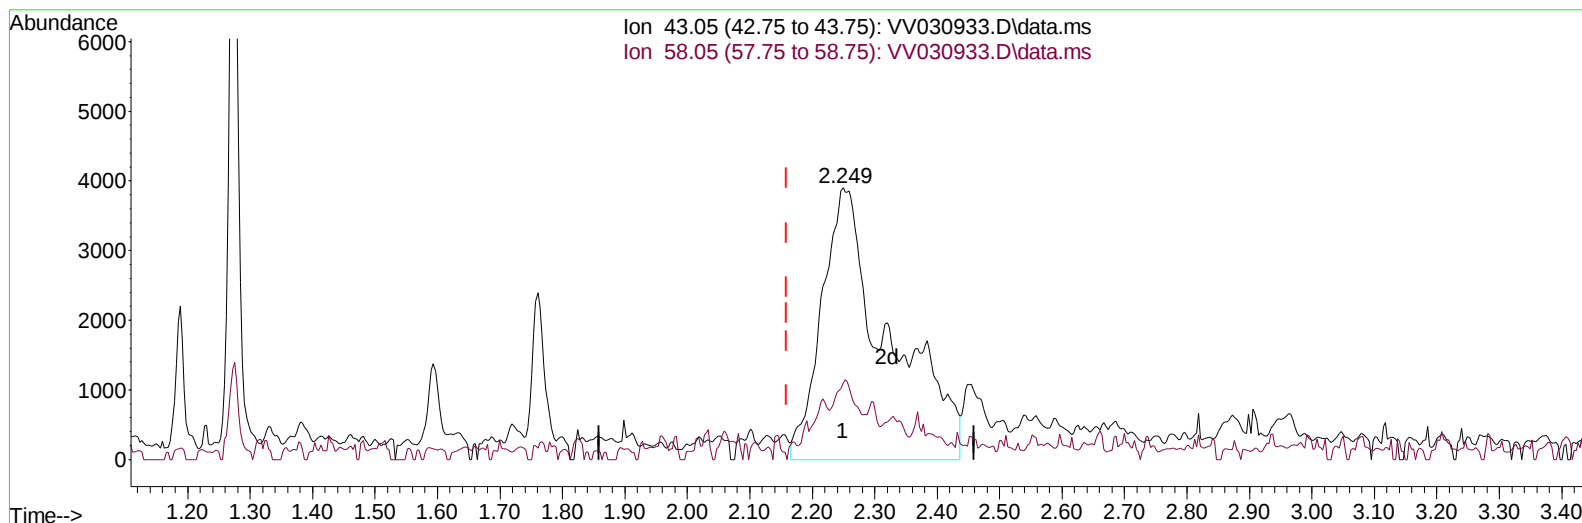

TIC: VV030933.D\data.ms

(13) Acetone (T)

2.249min (+ 0.090) 19.07 ug/L m

response 28963

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	18.50	7.01
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042823\
 Data File : VV030933.D
 Acq On : 28 Apr 2023 20:11
 Operator : SY/MD
 Sample : 02488-19
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHE74

Manual IntegrationsAPPROVED

Quant Time: Apr 29 01:13:24 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Apr 29 01:06:38 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/01/2023
 Supervised By :Mahesh Dadoda 05/01/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	121709	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	118066	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	62709	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	48890	4.876	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	97.600%	
7) Chloroethane-d5	1.529	69	42766	5.228	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	104.600%	
11) 1,1-Dichloroethene-d2	2.056	65	24840	4.681	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	93.600%	
20) 2-Butanone-d5	3.905	46	96936	54.514	ug/L	0.07
Spiked Amount 50.000	Range 40	- 130	Recovery	=	109.020%	
24) Chloroform-d	4.252	84	108791	5.459	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	109.200%	
26) 1,2-Dichloroethane-d4	4.950	65	50484	4.983	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	99.600%	
32) Benzene-d6	4.957	84	167230	4.832	ug/L	-0.02
Spiked Amount 5.000	Range 70	- 125	Recovery	=	96.600%	
36) 1,2-Dichloropropane-d6	5.995	67	48916	4.861	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	97.200%	
41) Toluene-d8	7.246	98	139573	4.235	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	84.800%	
43) trans-1,3-Dichloroprop...	7.564	79	14962	3.966	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	79.400%	
46) 2-Hexanone-d5	8.053	63	54518	41.250	ug/L	0.02
Spiked Amount 50.000	Range 45	- 130	Recovery	=	82.500%	
56) 1,1,2,2-Tetrachloroeth...	10.162	84	33366	4.574	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	91.400%	
66) 1,2-Dichlorobenzene-d4	11.567	152	59297	5.073	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	101.400%	
Target Compounds						
					Qvalue	
10) 1,1,2-Trichloro-1,2,2-...	2.063	101	3301	0.371	ug/L #	88
12) 1,1-Dichloroethene	2.066	96	64303	7.851	ug/L	86
13) Acetone	2.249	43	28963m	19.068	ug/L	
14) Carbon disulfide	2.236	76	111833	5.218	ug/L	100
19) 1,1-Dichloroethane	3.111	63	6261	0.433	ug/L	92
29) 1,1,1-Trichloroethane	4.506	97	25728	1.734	ug/L #	90
34) Trichloroethene	5.831	95	202908	25.631	ug/L	97
42) Toluene	7.320	91	147142	4.602	ug/L	100
47) Tetrachloroethene	7.908	164	60420	8.000	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042823\
Data File : VV030933.D
Acq On : 28 Apr 2023 20:11
Operator : SY/MD
Sample : 02488-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHE74

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 05/01/2023
Supervised By :Mahesh Dadoda 05/01/2023

Quant Time: Apr 29 01:13:24 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Apr 29 01:06:38 2023
Response via : Initial Calibration

