

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042823\
 Data File : VW030937.D
 Acq On : 28 Apr 2023 21:50
 Operator : SY/MD
 Sample : 02551-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHE78

Quant Time: Apr 29 01:14:52 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Apr 29 01:06:38 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.545	114	120832	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	119544	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	59446	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	47945	4.816	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	96.400%
7) Chloroethane-d5	1.539	69	44375	5.464	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	109.200%
11) 1,1-Dichloroethene-d2	2.066	65	25471	4.834	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	96.600%
20) 2-Butanone-d5	3.812	46	94539	53.552	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	107.100%
24) Chloroform-d	4.259	84	103475	5.230	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.600%
26) 1,2-Dichloroethane-d4	4.953	65	54887	5.457	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	109.200%
32) Benzene-d6	4.969	84	181950	5.192	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.800%
36) 1,2-Dichloropropane-d6	5.998	67	53529	5.254	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	105.000%
41) Toluene-d8	7.249	98	157446	4.718	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.400%
43) trans-1,3-Dichloroprop...	7.561	79	17960	4.702	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	94.000%
46) 2-Hexanone-d5	8.034	63	67028	50.089	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.180%
56) 1,1,2,2-Tetrachloroeth...	10.159	84	38269	5.182	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	103.600%
66) 1,2-Dichlorobenzene-d4	11.567	152	62135	5.607	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	112.200%
Target Compounds						
13) Acetone	2.140	43	3085	2.046	ug/L	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042823\
Data File : VV030937.D
Acq On : 28 Apr 2023 21:50
Operator : SY/MD
Sample : 02551-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHE78

Quant Time: Apr 29 01:14:52 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Apr 29 01:06:38 2023
Response via : Initial Calibration

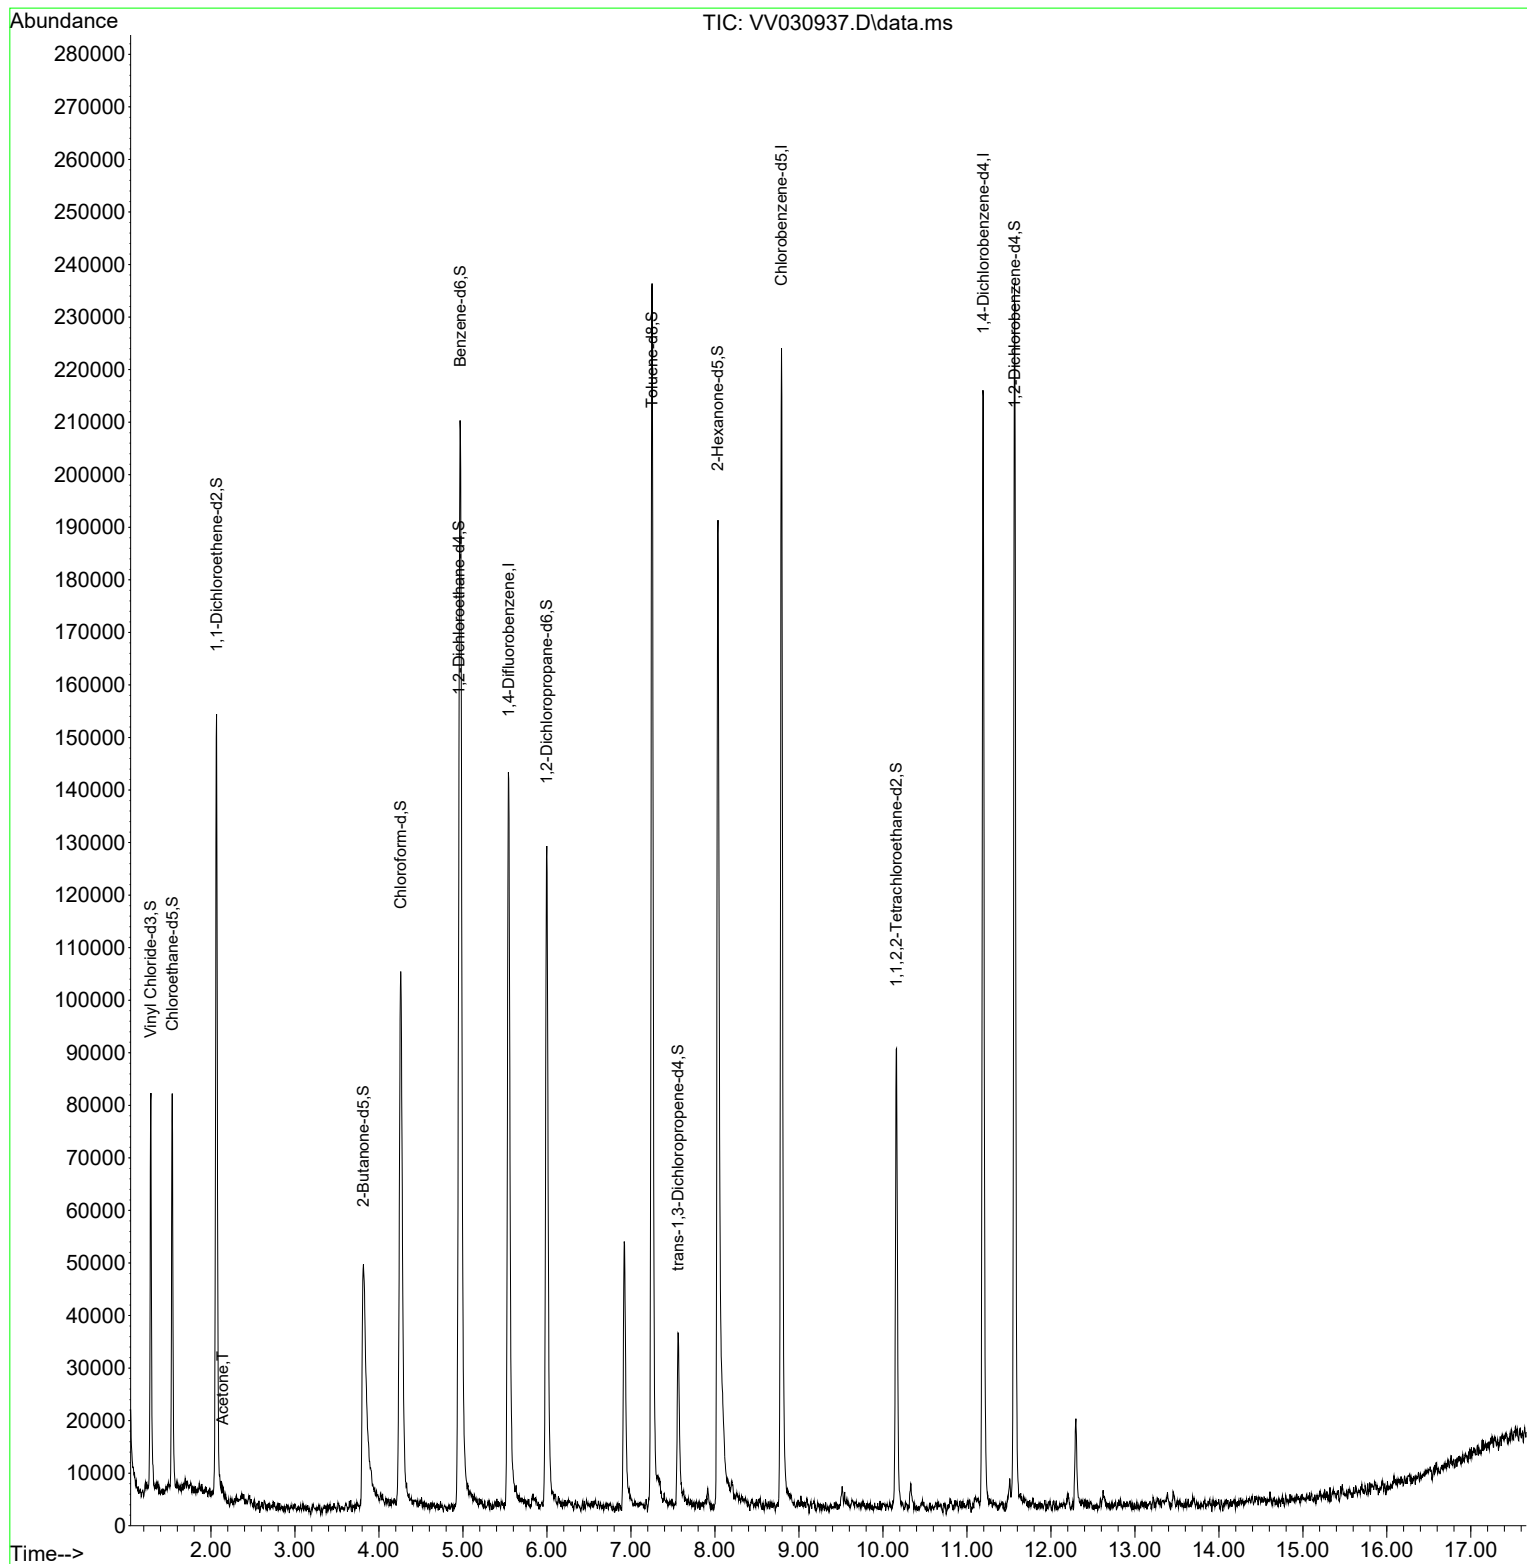

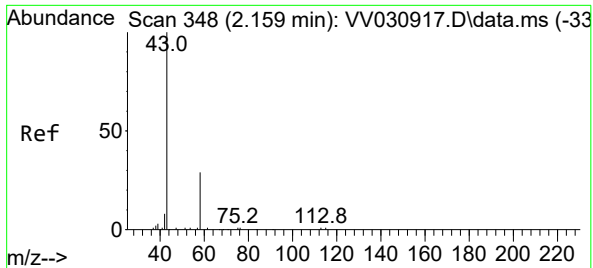

#13
 Acetone
 Concen: 2.046 ug/L
 RT: 2.140 min Scan# 34
 Delta R.T. -0.019 min
 Lab File: VV030937.D
 Acq: 28 Apr 2023 21:50

Instrument :
 MSVOA_V
 ClientSampleId :
 BHE78

Tgt Ion: 43 Resp: 3085
 Ion Ratio Lower Upper
 43 100
 58 26.2 0.0 37.0

