

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042823\
 Data File : VW030938.D
 Acq On : 28 Apr 2023 22:14
 Operator : SY/MD
 Sample : 02551-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHE79

Quant Time: Apr 29 01:15:11 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Apr 29 01:06:38 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.545	114	127893	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	126614	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	63455	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	49787	4.725	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	94.400%
7) Chloroethane-d5	1.539	69	44860	5.219	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	104.400%
11) 1,1-Dichloroethene-d2	2.066	65	24590	4.410	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	88.200%
20) 2-Butanone-d5	3.815	46	94940	50.810	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	101.620%
24) Chloroform-d	4.259	84	103325	4.934	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.600%
26) 1,2-Dichloroethane-d4	4.953	65	55687	5.231	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.600%
32) Benzene-d6	4.969	84	180246	4.857	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.200%
36) 1,2-Dichloropropane-d6	5.998	67	52671	4.881	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.600%
41) Toluene-d8	7.252	98	155785	4.408	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.200%
43) trans-1,3-Dichloroprop...	7.564	79	20047	4.956	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	99.200%
46) 2-Hexanone-d5	8.034	63	65350	46.108	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	92.220%
56) 1,1,2,2-Tetrachloroeth...	10.159	84	37718	4.822	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.400%
66) 1,2-Dichlorobenzene-d4	11.567	152	62044	5.245	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.000%
Target Compounds						Qvalue
13) Acetone	2.140	43	4484	2.809	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042823\
Data File : VV030938.D
Acq On : 28 Apr 2023 22:14
Operator : SY/MD
Sample : 02551-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHE79

Quant Time: Apr 29 01:15:11 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Apr 29 01:06:38 2023
Response via : Initial Calibration

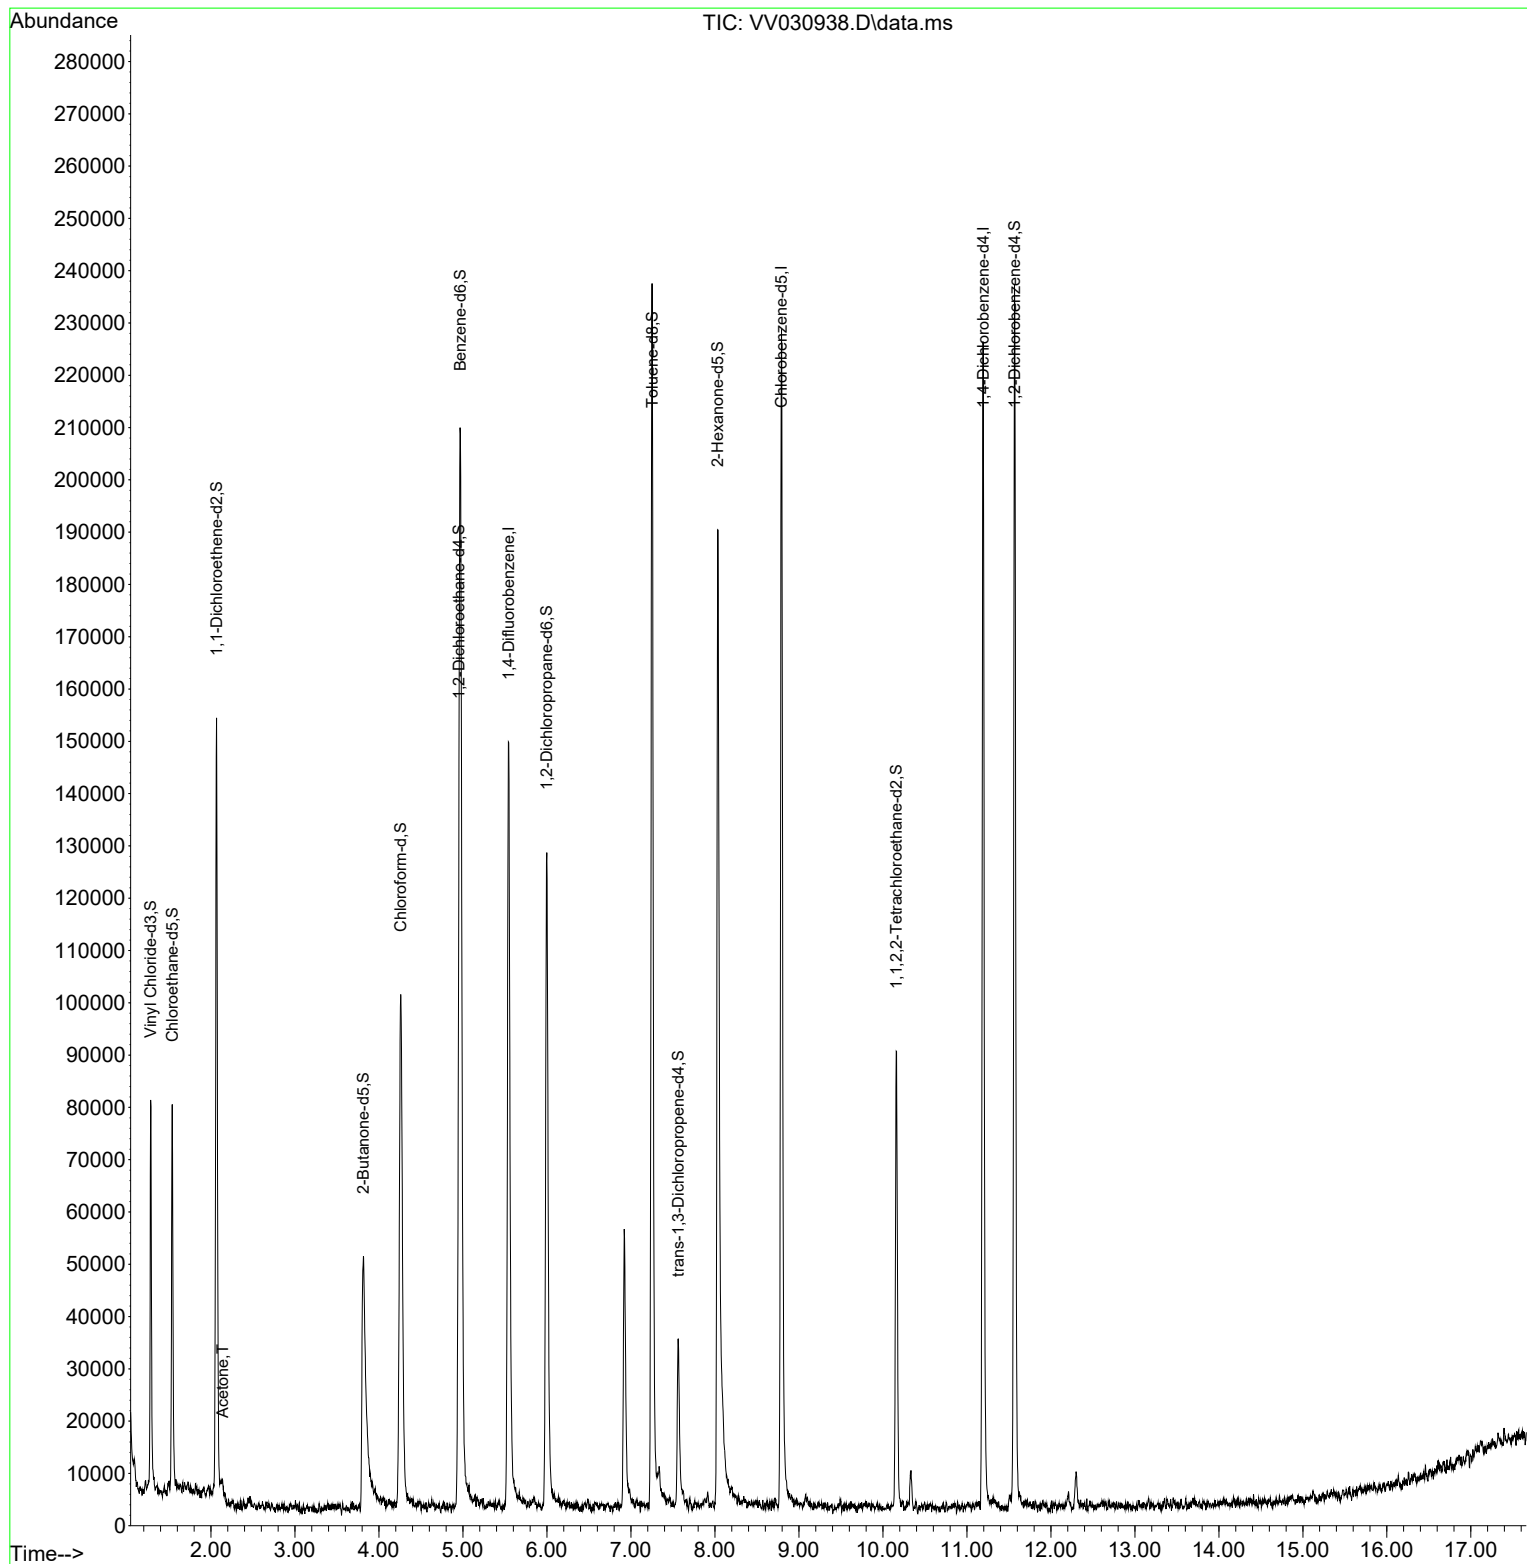

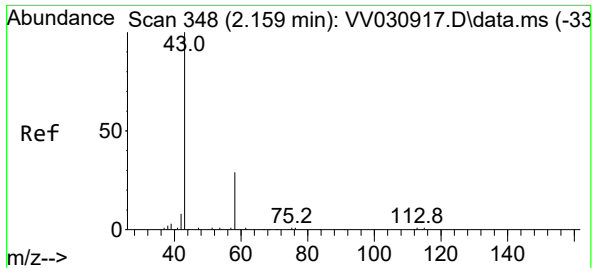

#13
 Acetone
 Concen: 2.809 ug/L
 RT: 2.140 min Scan# 34
 Delta R.T. -0.019 min
 Lab File: VV030938.D
 Acq: 28 Apr 2023 22:14

Instrument :
 MSVOA_V
 ClientSampleId :
 BHE79

Tgt Ion: 43 Resp: 4484
 Ion Ratio Lower Upper
 43 100
 58 15.7 0.0 37.0

