

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042823\
 Data File : VV030920.D
 Acq On : 28 Apr 2023 14:55
 Operator : SY/MD
 Sample : 02488-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHE62

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030920.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	86	rBV	76318	84992	15.72%	1.645%
2	1.536	147	154	170	rVB	70595	88884	16.44%	1.720%
3	2.063	309	318	332	rVB	166193	248660	46.00%	4.812%
4	3.828	854	867	891	rBV4	48675	180220	33.34%	3.488%
5	4.259	986	1001	1029	rBV	97945	277049	51.25%	5.362%
6	4.741	1138	1151	1163	rBV4	12387	29495	5.46%	0.571%
7	4.966	1204	1221	1243	rBV2	212730	540575	100.00%	10.462%
8	5.542	1386	1400	1418	rBV	167531	354798	65.63%	6.867%
9	5.841	1478	1493	1513	rBV	247671	504229	93.28%	9.759%
10	5.998	1530	1542	1558	rBV	119251	249519	46.16%	4.829%
11	6.921	1819	1829	1850	rBV	51945	101097	18.70%	1.957%
12	7.252	1920	1932	1949	rBV	238992	428590	79.28%	8.295%
13	7.561	2019	2028	2048	rBV3	31970	65793	12.17%	1.273%
14	7.912	2119	2137	2151	rBV3	92022	178962	33.11%	3.464%
15	8.040	2167	2177	2211	rBV	166754	402145	74.39%	7.783%
16	8.793	2400	2411	2430	rBV	253289	435098	80.49%	8.421%
17	10.162	2824	2837	2852	rBV	81700	137508	25.44%	2.661%
18	10.333	2877	2890	2903	rVB	38365	65284	12.08%	1.263%
19	11.194	3145	3158	3176	rBV	252219	401752	74.32%	7.775%
20	11.513	3248	3257	3260	rBV9	4646	7275	1.35%	0.141%
21	11.571	3263	3275	3292	rVB	227079	373661	69.12%	7.232%
22	12.204	3465	3472	3480	rVB4	8186	11457	2.12%	0.222%




Sum of corrected areas: 5167043

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042823\
Data File : VV030920.D
Acq On : 28 Apr 2023 14:55
Operator : SY/MD
Sample : 02488-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHE62

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

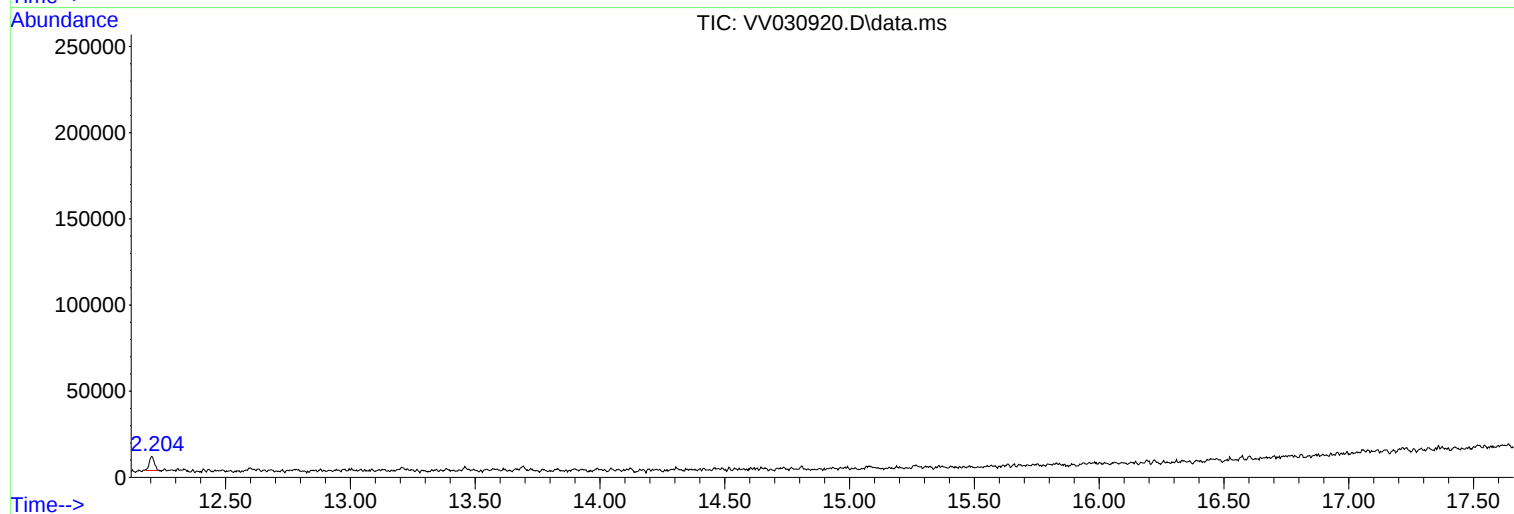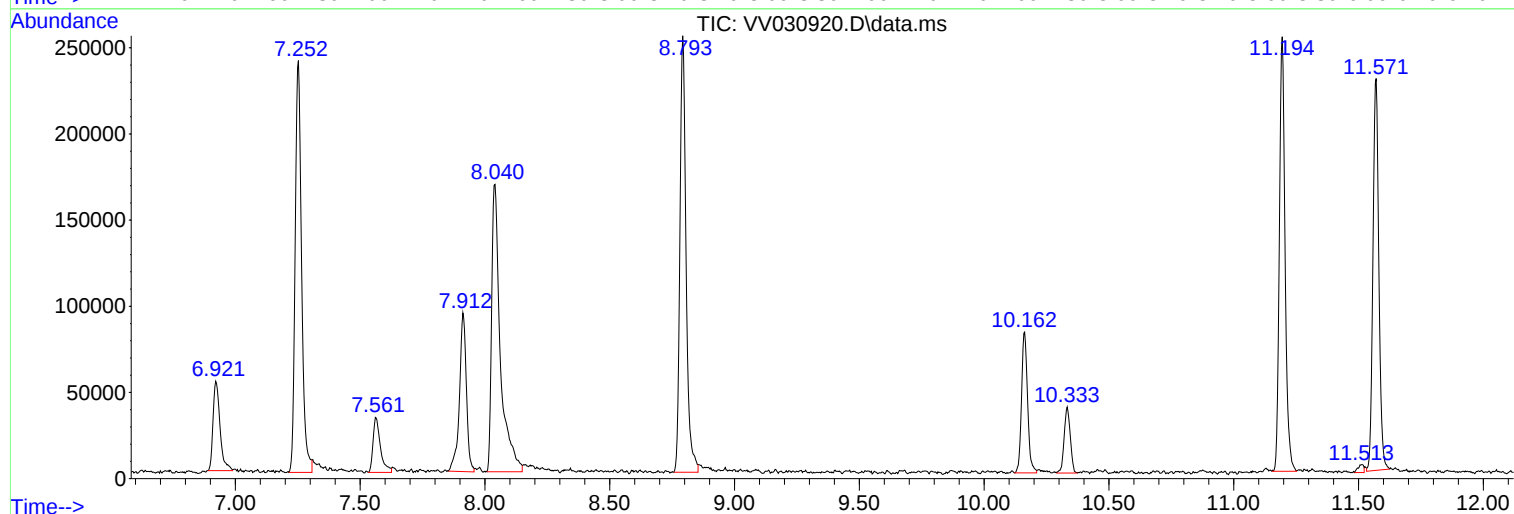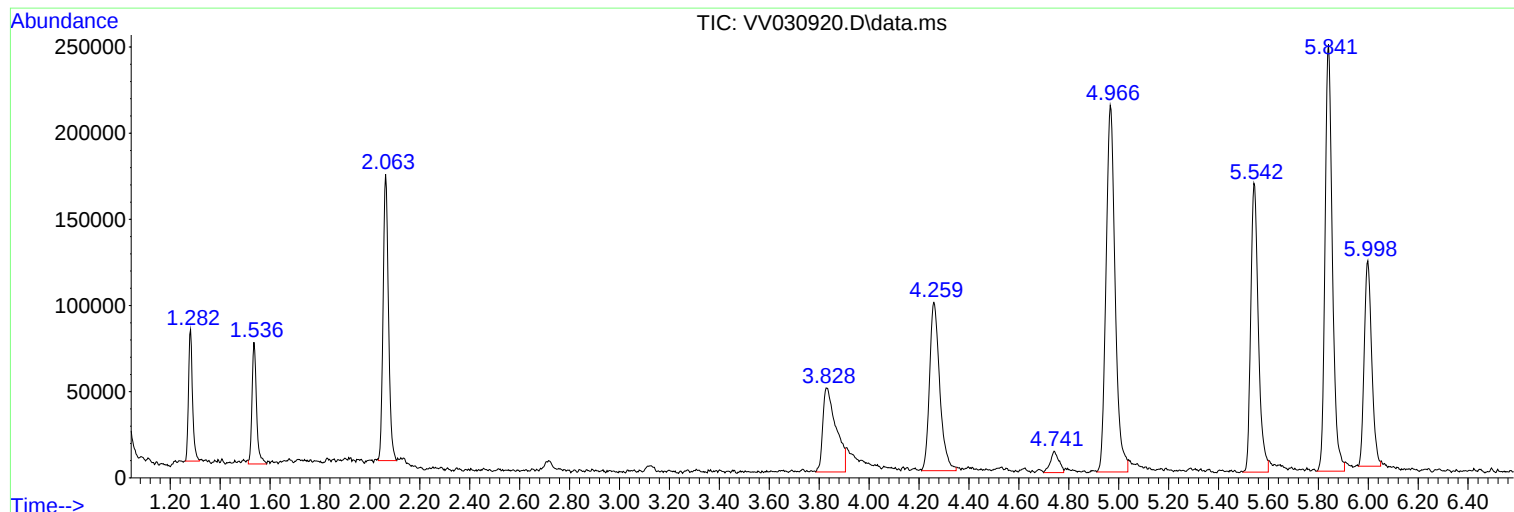

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042823\
Data File : VV030920.D
Acq On : 28 Apr 2023 14:55
Operator : SY/MD
Sample : 02488-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHE62

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042823\
Data File : VV030920.D
Acq On : 28 Apr 2023 14:55
Operator : SY/MD
Sample : 02488-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHE62

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc