

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042823\
 Data File : VV030921.D
 Acq On : 28 Apr 2023 15:19
 Operator : SY/MD
 Sample : 02488-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHE68

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030921.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	83	rBV	83867	88317	15.02%	1.914%
2	1.535	148	154	166	rVB	77359	88116	14.99%	1.910%
3	2.063	307	318	333	rBV	172437	257618	43.82%	5.583%
4	3.834	855	869	892	rBV2	36682	150604	25.62%	3.264%
5	4.262	985	1002	1028	rBV	106701	284597	48.41%	6.168%
6	4.966	1202	1221	1243	rBV2	229572	587901	100.00%	12.741%
7	5.542	1387	1400	1424	rBV	153874	328530	55.88%	7.120%
8	5.850	1484	1496	1502	rBV	5829	11357	1.93%	0.246%
9	5.998	1527	1542	1566	rBV	132468	284098	48.32%	6.157%
10	6.921	1817	1829	1846	rBV	58448	116742	19.86%	2.530%
11	7.252	1920	1932	1949	rBV	259631	465832	79.24%	10.096%
12	7.564	2019	2029	2047	rBV3	34720	66260	11.27%	1.436%
13	7.915	2120	2138	2149	rBV3	42195	80844	13.75%	1.752%
14	8.037	2166	2176	2210	rBV	191852	442522	75.27%	9.591%
15	8.792	2400	2411	2426	rBV	236690	400686	68.16%	8.684%
16	10.162	2826	2837	2851	rBV	90804	149626	25.45%	3.243%
17	10.332	2879	2890	2903	rBV	16930	31047	5.28%	0.673%
18	11.194	3146	3158	3177	rBV	228317	376646	64.07%	8.163%
19	11.567	3263	3274	3294	rBV	241746	402763	68.51%	8.729%




Sum of corrected areas: 4614106

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042823\
Data File : VV030921.D
Acq On : 28 Apr 2023 15:19
Operator : SY/MD
Sample : 02488-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHE68

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

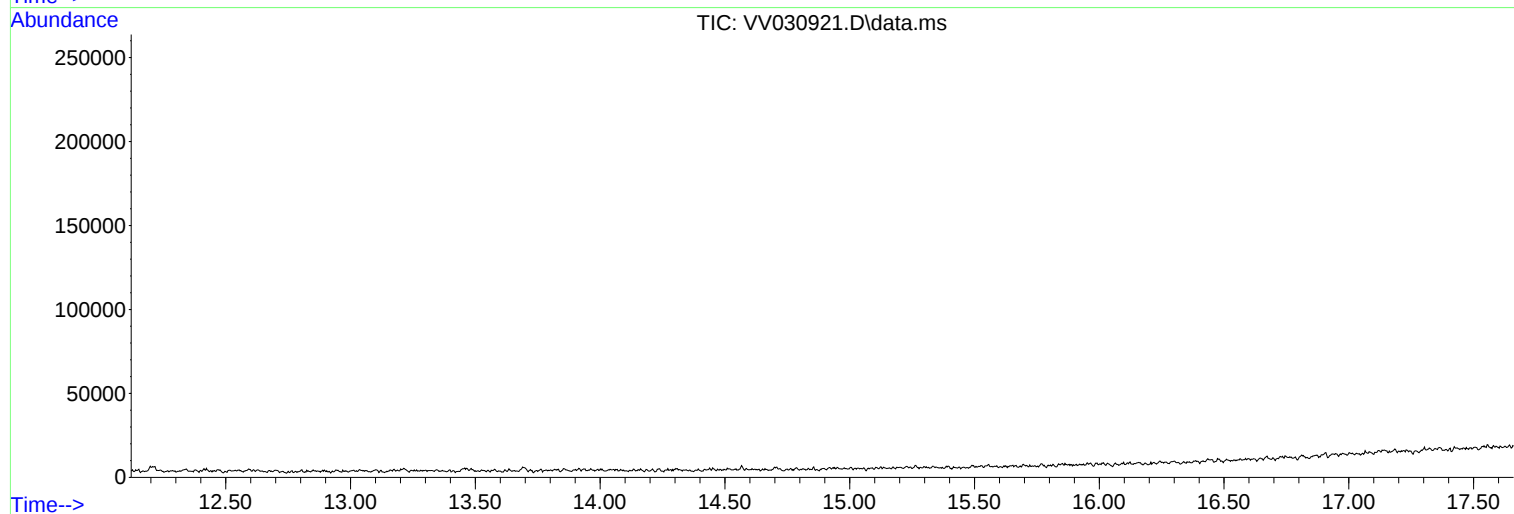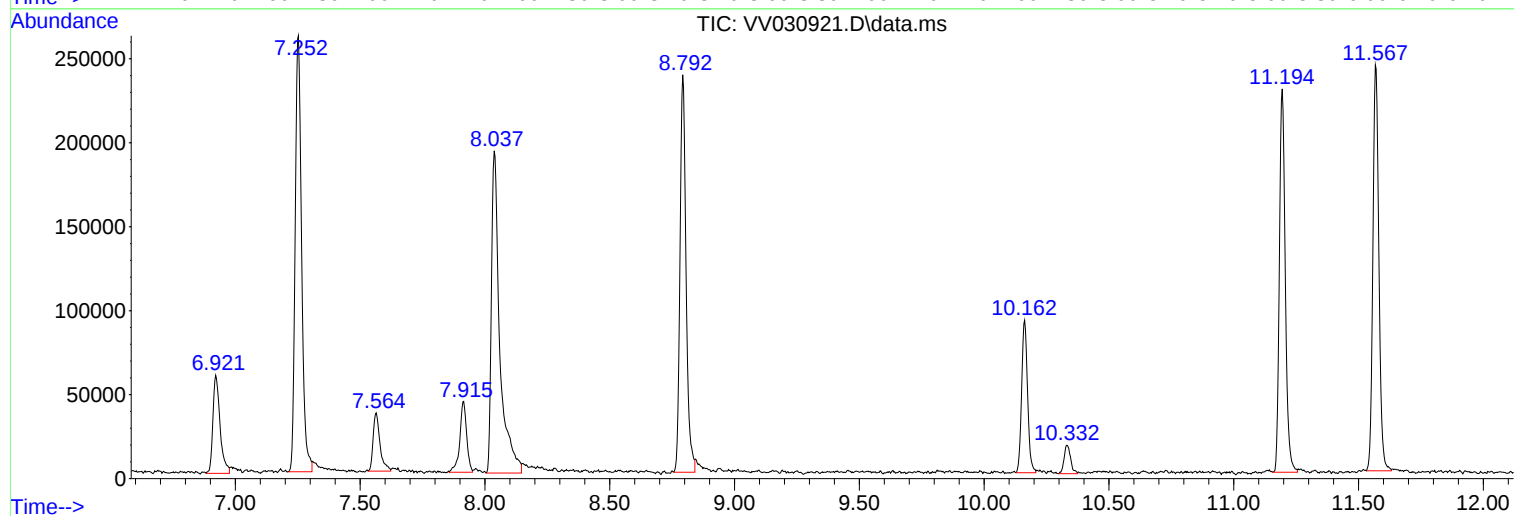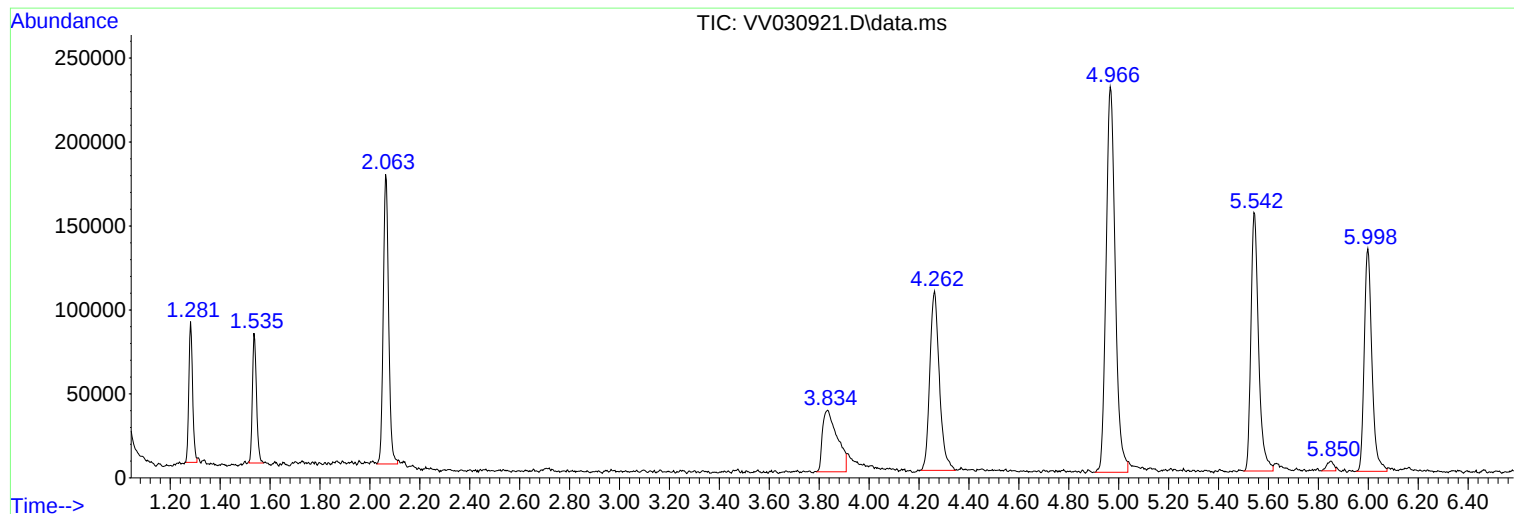

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042823\
Data File : VV030921.D
Acq On : 28 Apr 2023 15:19
Operator : SY/MD
Sample : 02488-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHE68

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042823\
Data File : VV030921.D
Acq On : 28 Apr 2023 15:19
Operator : SY/MD
Sample : 02488-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHE68

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc