

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042823\
 Data File : VV030922.D
 Acq On : 28 Apr 2023 15:44
 Operator : SY/MD
 Sample : 02488-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHE70

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030922.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	84	rBV	83212	88998	15.65%	2.042%
2	1.535	147	154	165	rVB	76443	89443	15.73%	2.053%
3	2.063	309	318	330	rVV	169572	242951	42.72%	5.575%
4	3.841	857	871	886	rBV2	31529	115781	20.36%	2.657%
5	4.259	981	1001	1025	rBV	103426	270243	47.52%	6.202%
6	4.966	1204	1221	1246	rBV4	221296	568738	100.00%	13.052%
7	5.545	1387	1401	1419	rBV	143809	305731	53.76%	7.016%
8	5.998	1528	1542	1561	rBV	130603	272234	47.87%	6.247%
9	6.921	1818	1829	1850	rBV	55639	117014	20.57%	2.685%
10	7.252	1918	1932	1948	rBV	248898	455282	80.05%	10.448%
11	7.561	2019	2028	2042	rBV2	34489	66231	11.65%	1.520%
12	8.037	2165	2176	2215	rBV	179857	439826	77.33%	10.093%
13	8.792	2397	2411	2437	rBV	220202	389694	68.52%	8.943%
14	10.162	2825	2837	2849	rBV	90732	146967	25.84%	3.373%
15	10.336	2887	2891	2897	rVB6	5691	6599	1.16%	0.151%
16	11.194	3144	3158	3174	rBV	214649	362450	63.73%	8.318%
17	11.567	3263	3274	3292	rVB	242623	395299	69.50%	9.071%
18	12.204	3465	3472	3477	rBV8	4230	6113	1.07%	0.140%
19	12.300	3493	3502	3517	rVB8	10865	18021	3.17%	0.414%




Sum of corrected areas: 4357615

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042823\
Data File : VV030922.D
Acq On : 28 Apr 2023 15:44
Operator : SY/MD
Sample : 02488-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHE70

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

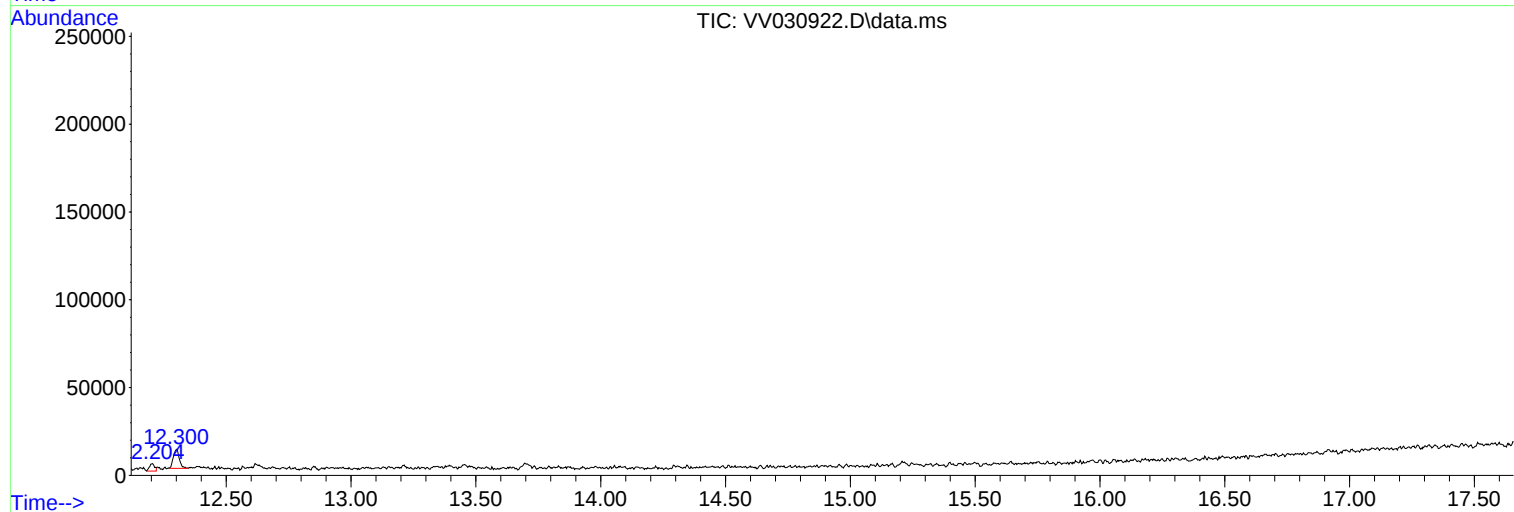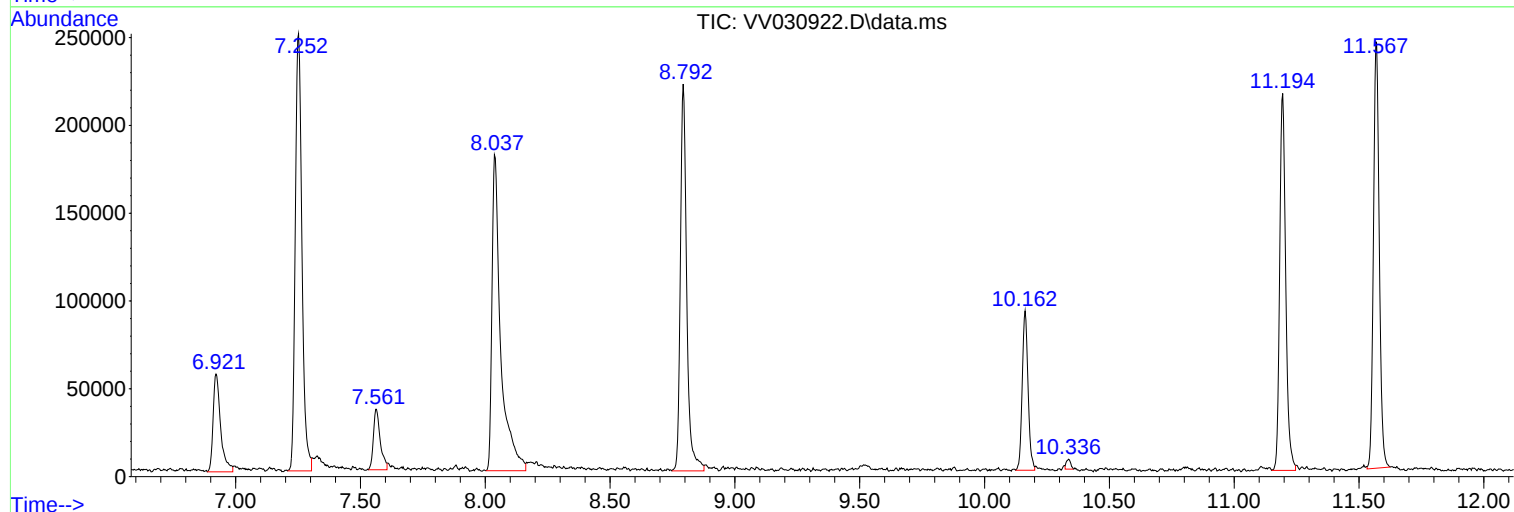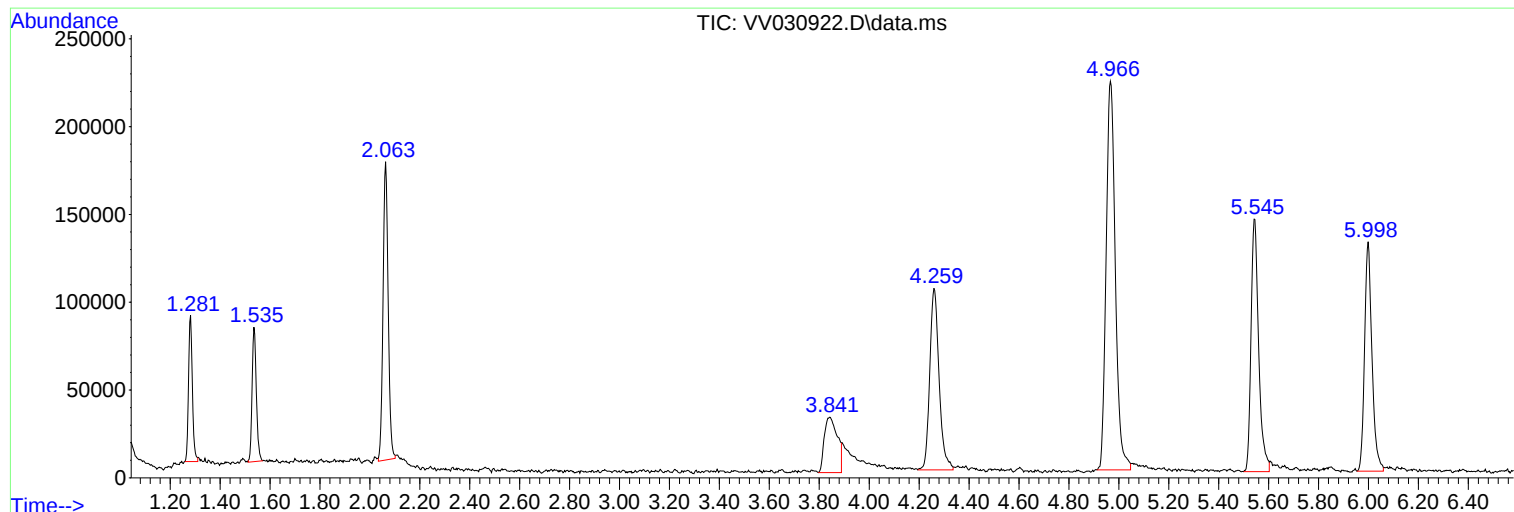

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042823\
Data File : VV030922.D
Acq On : 28 Apr 2023 15:44
Operator : SY/MD
Sample : 02488-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHE70

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042823\
Data File : VV030922.D
Acq On : 28 Apr 2023 15:44
Operator : SY/MD
Sample : 02488-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHE70

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------