

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042823\
 Data File : VV030924.D
 Acq On : 28 Apr 2023 16:31
 Operator : SY/MD
 Sample : 02488-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHE72

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030924.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	67	75	84	rBV	87601	96949	16.81%	2.198%
2	1.535	145	154	170	rBV	76831	93123	16.15%	2.111%
3	2.063	309	318	333	rVB	164717	237139	41.13%	5.375%
4	3.841	857	871	884	rBV	27261	94026	16.31%	2.131%
5	4.262	987	1002	1023	rBV	101782	259848	45.07%	5.890%
6	4.969	1204	1222	1248	rBV2	221192	576596	100.00%	13.070%
7	5.545	1389	1401	1421	rBV	144220	309897	53.75%	7.025%
8	5.998	1528	1542	1562	rBV2	127141	276141	47.89%	6.259%
9	6.924	1819	1830	1848	rBV2	54277	112383	19.49%	2.547%
10	7.252	1920	1932	1949	rBV	248304	449405	77.94%	10.187%
11	7.326	1953	1955	1963	rVB8	4512	5967	1.03%	0.135%
12	7.564	2019	2029	2043	rBV2	33615	65977	11.44%	1.496%
13	8.040	2164	2177	2209	rBV	201007	489369	84.87%	11.093%
14	8.792	2396	2411	2435	rBV	223142	393210	68.20%	8.913%
15	10.162	2824	2837	2854	rBV2	96033	159319	27.63%	3.611%
16	10.336	2881	2891	2897	rBV4	9264	14671	2.54%	0.333%
17	11.194	3147	3158	3176	rBV	226953	365022	63.31%	8.274%
18	11.570	3262	3275	3293	rVB	245767	403245	69.94%	9.141%
19	12.303	3494	3503	3508	rBV10	5558	9342	1.62%	0.212%




Sum of corrected areas: 4411629

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042823\
Data File : VV030924.D
Acq On : 28 Apr 2023 16:31
Operator : SY/MD
Sample : 02488-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHE72

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

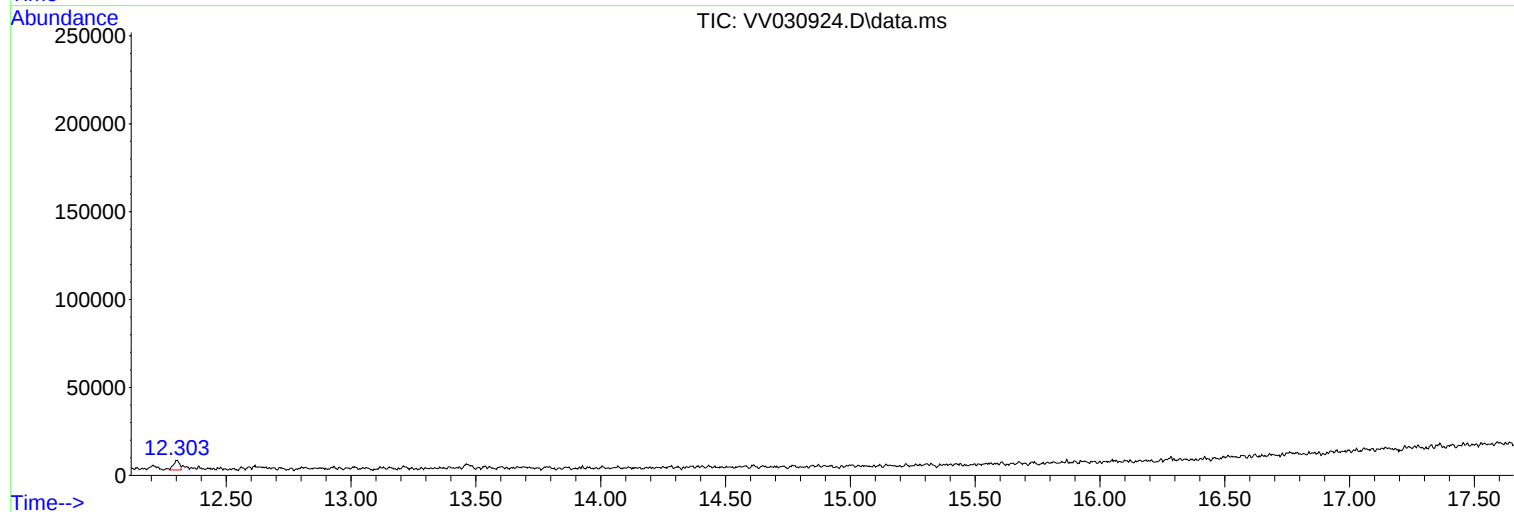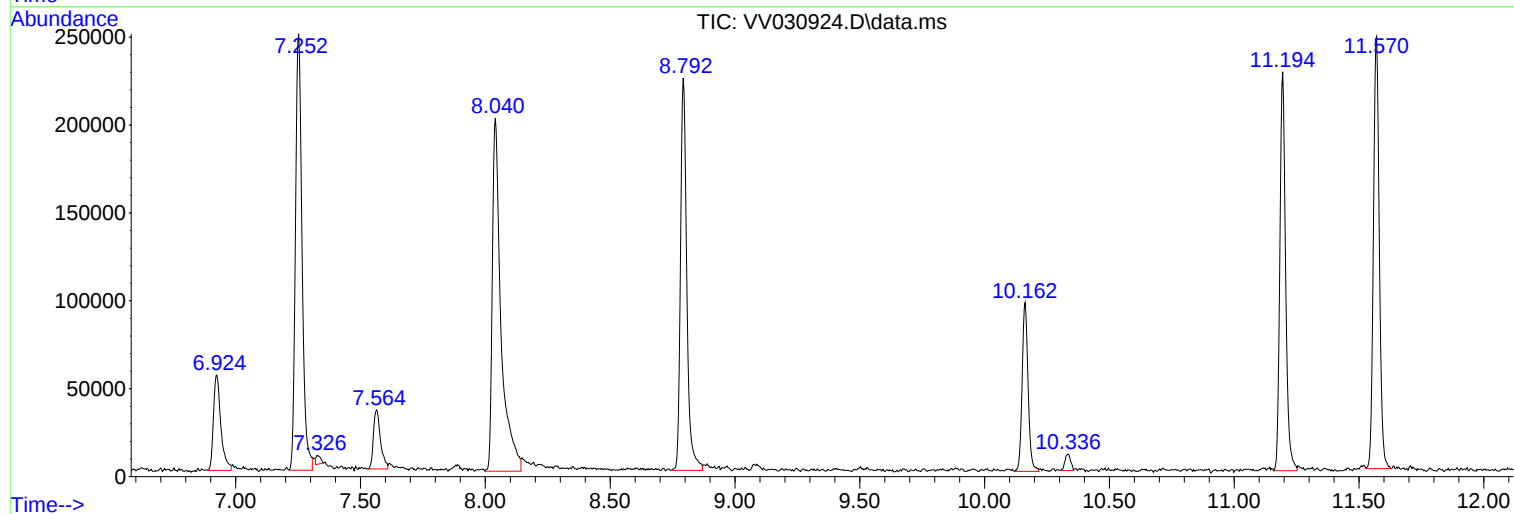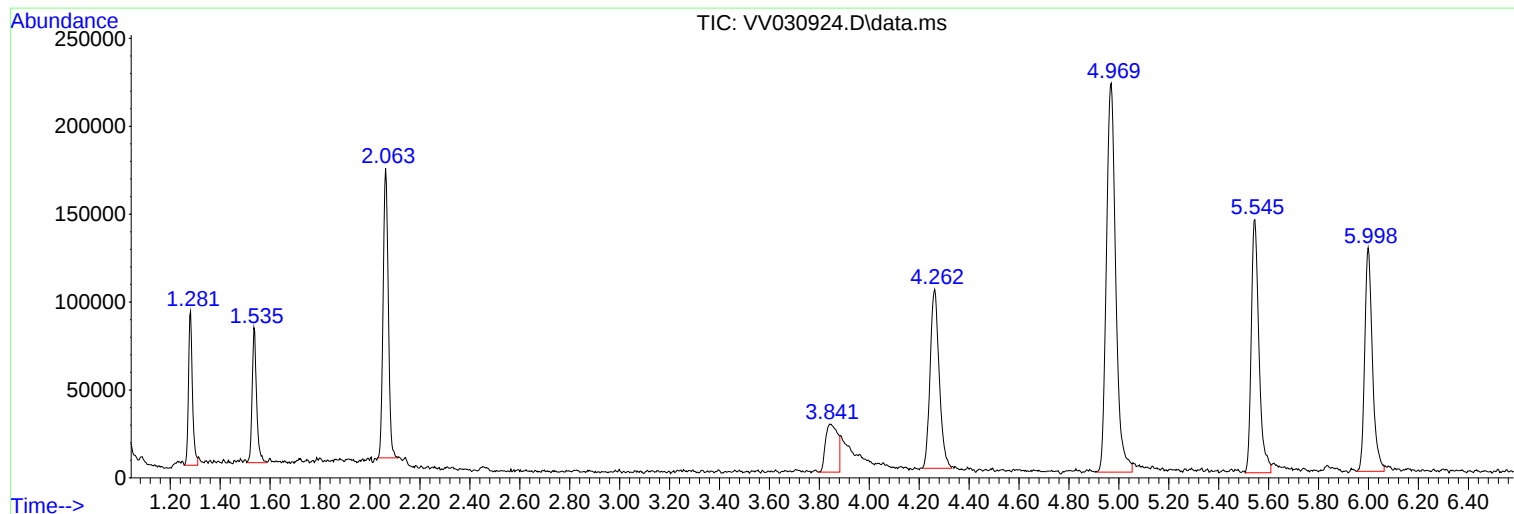

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042823\
Data File : VV030924.D
Acq On : 28 Apr 2023 16:31
Operator : SY/MD
Sample : 02488-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHE72

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042823\
Data File : VV030924.D
Acq On : 28 Apr 2023 16:31
Operator : SY/MD
Sample : 02488-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHE72

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------