

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042823\
 Data File : VV030925.D
 Acq On : 28 Apr 2023 16:54
 Operator : SY/MD
 Sample : 02488-14DL 250X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHE69DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030925.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	88	rBV	70940	77481	13.44%	1.673%
2	1.535	147	154	166	rVB	68012	78476	13.62%	1.695%
3	2.063	308	318	330	rBV	150277	216439	37.55%	4.675%
4	2.455	431	440	450	rVB3	10908	17608	3.05%	0.380%
5	3.847	860	873	898	rBV2	27191	128096	22.22%	2.767%
6	4.262	984	1002	1020	rBV2	89372	234946	40.76%	5.074%
7	4.969	1206	1222	1245	rBV2	194232	500478	86.83%	10.809%
8	5.545	1387	1401	1421	rBV	142360	309193	53.64%	6.678%
9	5.847	1481	1495	1507	rBV4	19879	43935	7.62%	0.949%
10	5.998	1529	1542	1560	rBV2	113061	237084	41.13%	5.120%
11	6.924	1819	1830	1845	rBV2	49353	97226	16.87%	2.100%
12	7.252	1919	1932	1955	rBV	216046	396697	68.82%	8.568%
13	7.564	2020	2029	2047	rBV2	31579	59123	10.26%	1.277%
14	7.911	2123	2137	2160	rBV	326662	576387	100.00%	12.449%
15	8.040	2165	2177	2209	rBV	184350	428857	74.40%	9.262%
16	8.792	2397	2411	2433	rBV	216239	376811	65.37%	8.138%
17	10.162	2826	2837	2851	rBV	85765	143365	24.87%	3.096%
18	11.194	3148	3158	3174	rBV	219296	348678	60.49%	7.531%
19	11.570	3258	3275	3289	rBV	219004	359251	62.33%	7.759%




Sum of corrected areas: 4630131

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042823\
Data File : VV030925.D
Acq On : 28 Apr 2023 16:54
Operator : SY/MD
Sample : 02488-14DL 250X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHE69DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

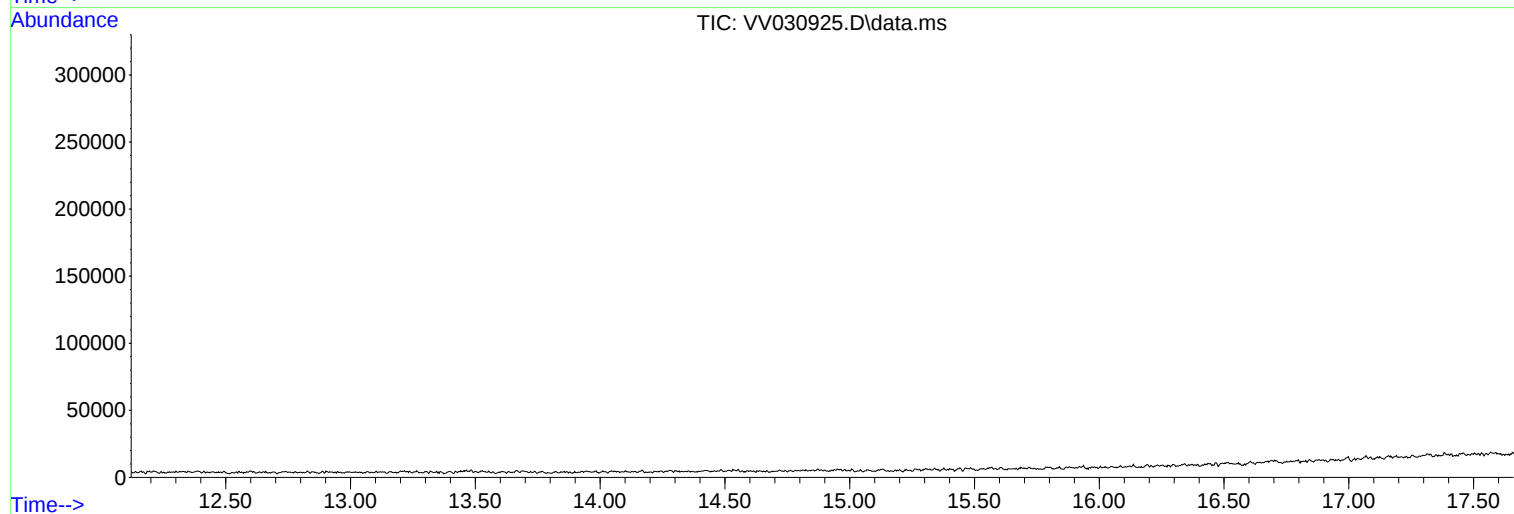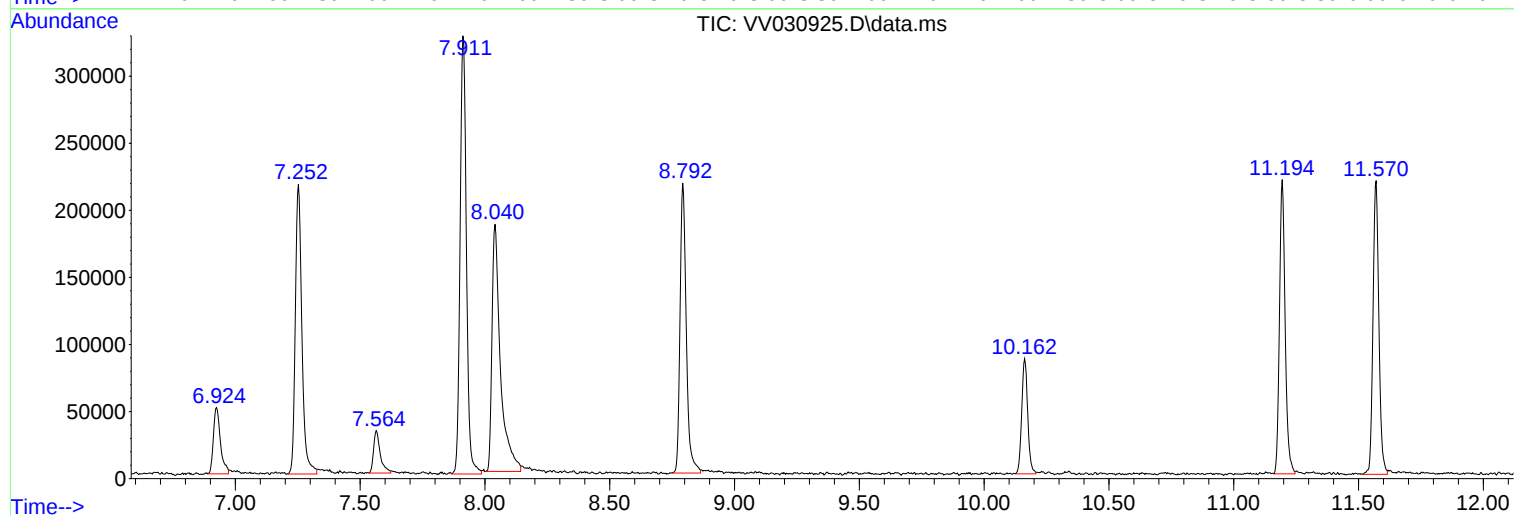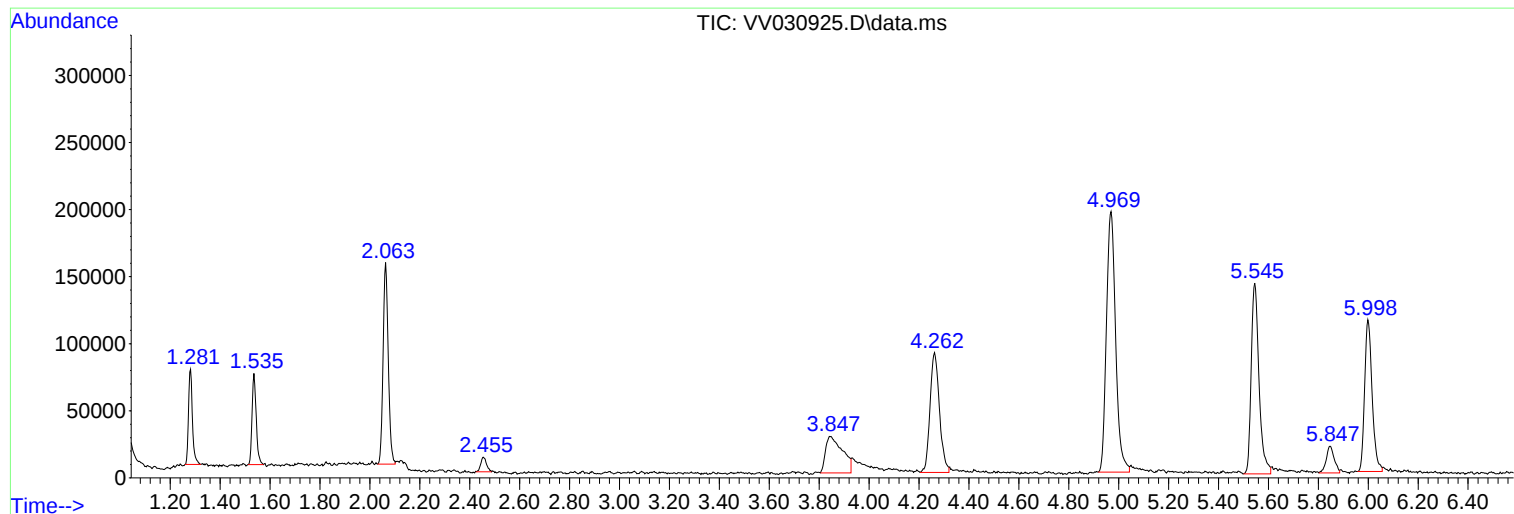

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042823\
Data File : VV030925.D
Acq On : 28 Apr 2023 16:54
Operator : SY/MD
Sample : 02488-14DL 250X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHE69DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042823\
Data File : VV030925.D
Acq On : 28 Apr 2023 16:54
Operator : SY/MD
Sample : 02488-14DL 250X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHE69DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc