

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042823\
 Data File : VV030927.D
 Acq On : 28 Apr 2023 17:43
 Operator : SY/MD
 Sample : 02488-12 20X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHE67

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030927.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	65	75	84	rBV	70124	78395	14.35%	1.744%
2	1.535	146	154	165	rVV	67012	81676	14.95%	1.817%
3	2.063	308	318	333	rBV	145038	211895	38.79%	4.713%
4	2.133	338	340	347	rVB8	7407	7419	1.36%	0.165%
5	2.455	432	440	449	rBV5	10149	15906	2.91%	0.354%
6	3.838	860	870	875	rBV	26055	51797	9.48%	1.152%
7	4.259	985	1001	1022	rBV2	90371	235043	43.03%	5.228%
8	4.966	1205	1221	1245	rBV3	195084	506295	92.69%	11.262%
9	5.542	1387	1400	1420	rBV	143592	305973	56.02%	6.806%
10	5.847	1480	1495	1510	rBV	11500	28402	5.20%	0.632%
11	5.998	1527	1542	1563	rBV	114289	247860	45.38%	5.513%
12	6.924	1817	1830	1848	rBV2	50675	101893	18.65%	2.266%
13	7.252	1918	1932	1948	rBV	215192	385194	70.52%	8.568%
14	7.564	2017	2029	2038	rBV2	33346	59646	10.92%	1.327%
15	7.911	2125	2137	2154	rBV	319936	546209	100.00%	12.150%
16	8.040	2167	2177	2208	rBV	168465	413672	75.74%	9.202%
17	8.792	2400	2411	2437	rBV	216746	375498	68.75%	8.352%
18	10.159	2825	2836	2851	rBV	87278	144329	26.42%	3.210%
19	11.194	3144	3158	3175	rBV	216532	345554	63.26%	7.686%
20	11.570	3261	3275	3288	rBV	212480	352990	64.63%	7.852%




Sum of corrected areas: 4495646

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042823\
Data File : VV030927.D
Acq On : 28 Apr 2023 17:43
Operator : SY/MD
Sample : 02488-12 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHE67

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

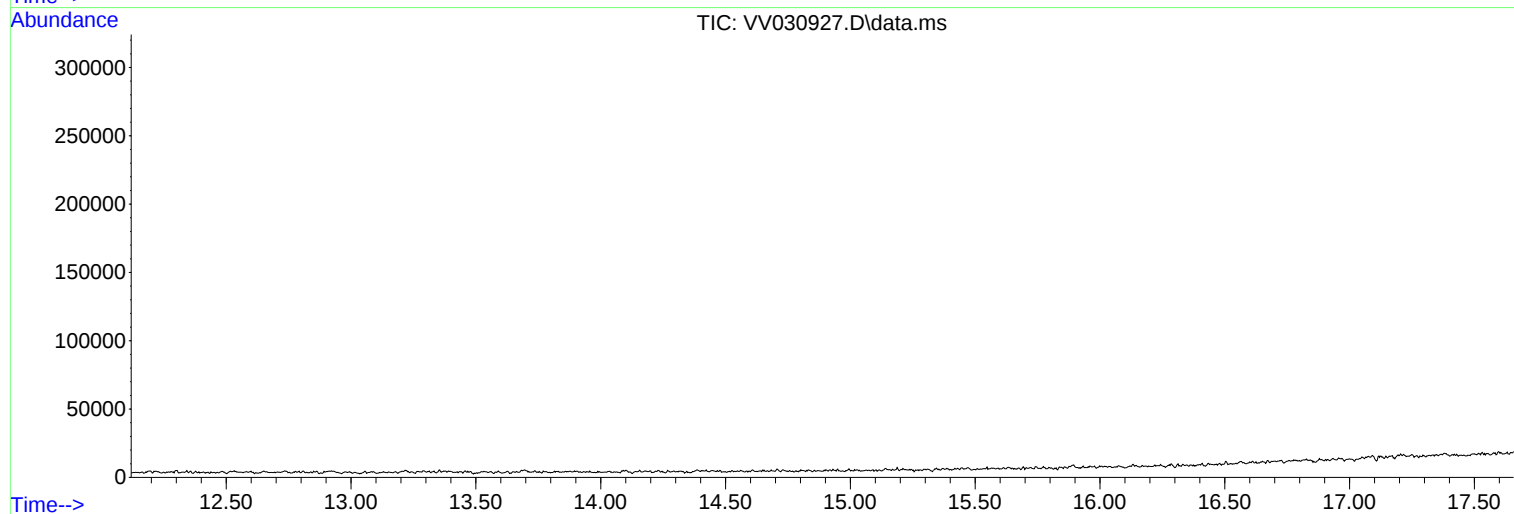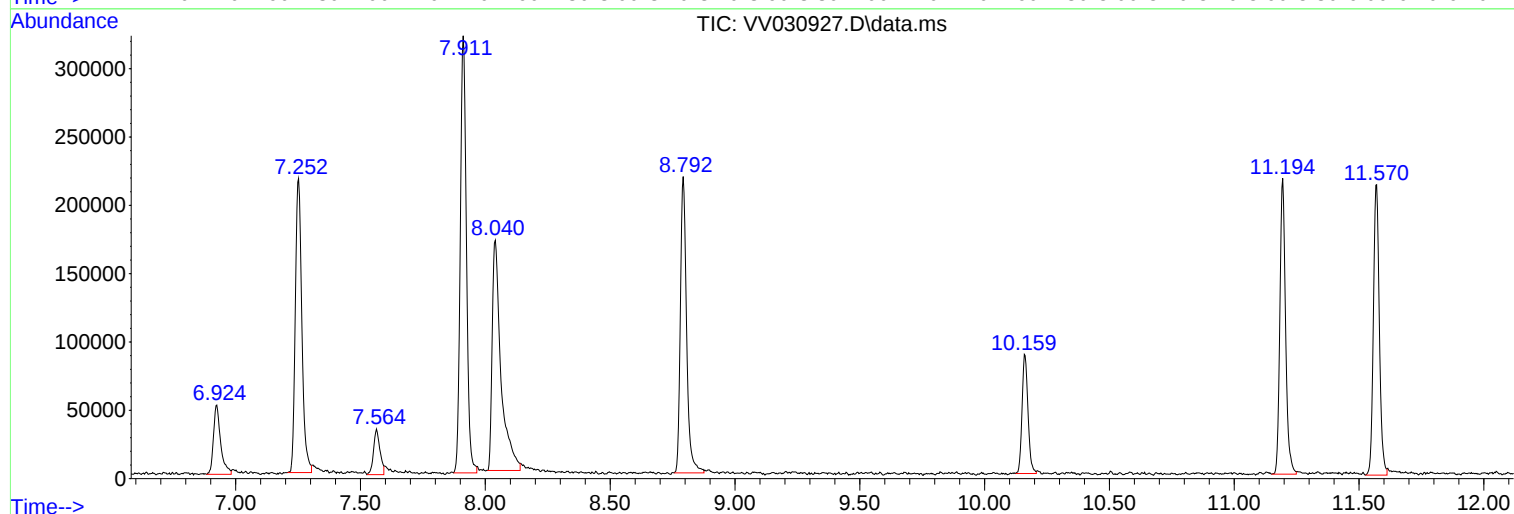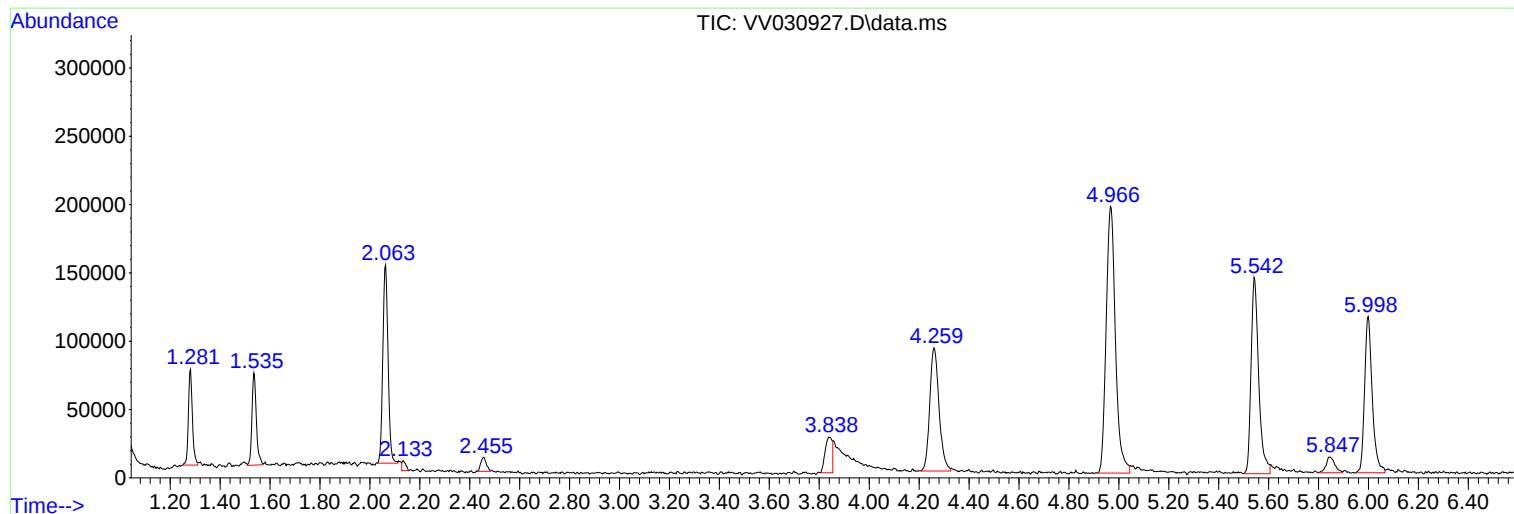

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042823\
Data File : VV030927.D
Acq On : 28 Apr 2023 17:43
Operator : SY/MD
Sample : 02488-12 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHE67

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042823\
Data File : VV030927.D
Acq On : 28 Apr 2023 17:43
Operator : SY/MD
Sample : 02488-12 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHE67

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc