

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042823\
 Data File : VV030929.D
 Acq On : 28 Apr 2023 18:32
 Operator : SY/MD
 Sample : 02488-18DL 5X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHE73DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030929.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.089	11	15	27	rVB3	13939	19856	4.11%	0.449%
2	1.282	66	75	86	rBV	74969	92584	19.15%	2.092%
3	1.536	147	154	166	rVB	61901	75118	15.54%	1.698%
4	2.066	307	319	331	rBV3	170195	277643	57.43%	6.275%
5	2.243	367	374	385	rVB2	20162	30759	6.36%	0.695%
6	2.455	431	440	449	rVB2	8704	14902	3.08%	0.337%
7	3.834	859	869	870	rBV2	26120	33607	6.95%	0.760%
8	4.259	986	1001	1024	rBV	88137	231425	47.87%	5.230%
9	4.519	1074	1082	1083	rBV6	6057	6453	1.33%	0.146%
10	4.966	1205	1221	1244	rBV3	186921	483420	100.00%	10.925%
11	5.542	1387	1400	1420	rBV	147821	315569	65.28%	7.132%
12	5.841	1479	1493	1518	rBV2	117218	252492	52.23%	5.706%
13	5.998	1527	1542	1563	rBV2	112219	238911	49.42%	5.399%
14	6.924	1819	1830	1850	rBV2	46110	93576	19.36%	2.115%
15	7.252	1921	1932	1947	rBV	209595	378690	78.34%	8.558%
16	7.326	1947	1955	1968	rVB	39448	74972	15.51%	1.694%
17	7.564	2021	2029	2047	rBV3	28283	52748	10.91%	1.192%
18	7.915	2126	2138	2154	rVB	54359	96300	19.92%	2.176%
19	8.040	2163	2177	2212	rBV	155606	383805	79.39%	8.674%
20	8.792	2400	2411	2434	rBV	231072	394357	81.58%	8.912%
21	9.764	2704	2713	2722	rBV	6584	11011	2.28%	0.249%
22	10.162	2827	2837	2849	rBV	77349	127722	26.42%	2.886%
23	10.995	3085	3096	3108	rBV2	15094	28906	5.98%	0.653%
24	11.194	3147	3158	3177	rBV	225568	369788	76.49%	8.357%
25	11.571	3262	3275	3287	rBV	208793	340250	70.38%	7.690%




Sum of corrected areas: 4424864

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042823\
Data File : VV030929.D
Acq On : 28 Apr 2023 18:32
Operator : SY/MD
Sample : 02488-18DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHE73DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

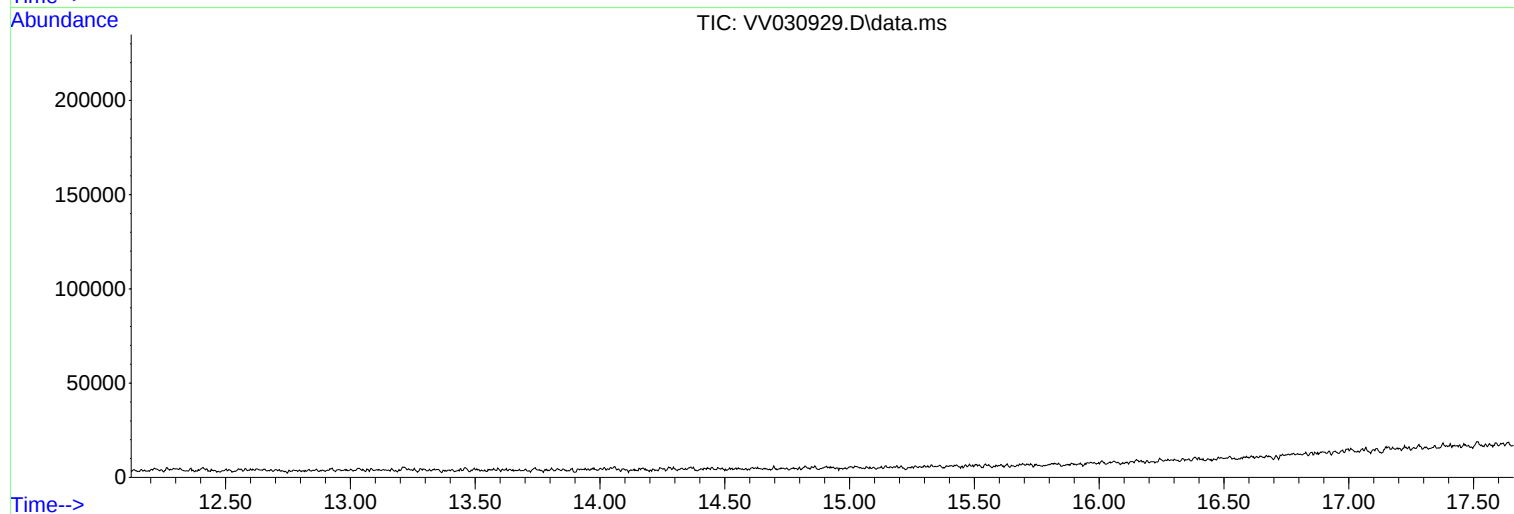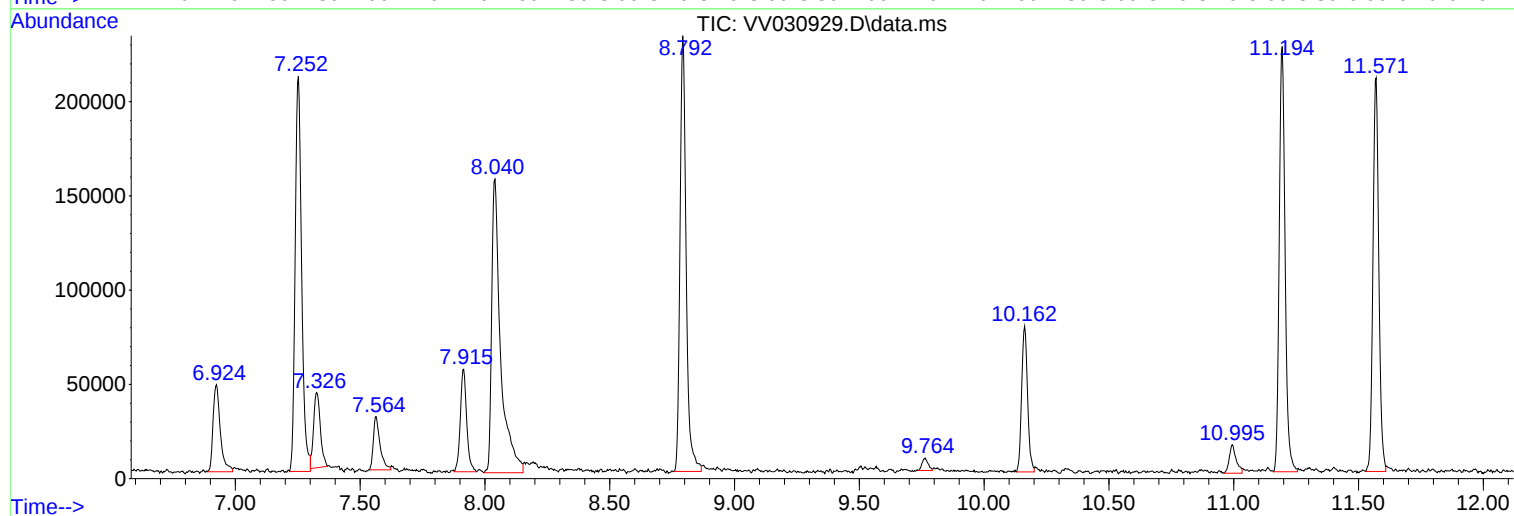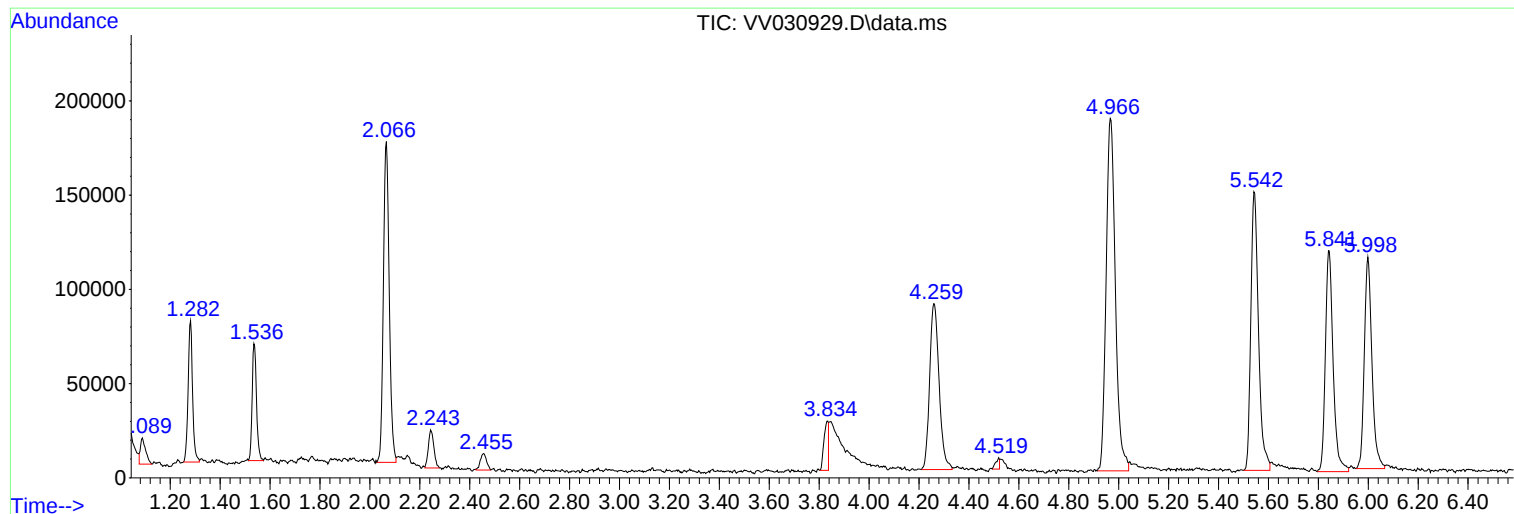

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042823\
Data File : VV030929.D
Acq On : 28 Apr 2023 18:32
Operator : SY/MD
Sample : 02488-18DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHE73DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042823\
Data File : VV030929.D
Acq On : 28 Apr 2023 18:32
Operator : SY/MD
Sample : 02488-18DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHE73DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc