

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042823\
 Data File : VV030930.D
 Acq On : 28 Apr 2023 18:57
 Operator : SY/MD
 Sample : 02488-19DL 5X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHE74DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030930.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.088	11	15	31	rVB2	12119	19058	3.78%	0.429%
2	1.281	66	75	87	rBV	76095	93167	18.47%	2.095%
3	1.535	147	154	163	rBV	64924	76190	15.10%	1.713%
4	2.066	309	319	332	rBV3	171108	275442	54.61%	6.194%
5	2.243	367	374	387	rVB	15842	26635	5.28%	0.599%
6	2.455	431	440	451	rBV3	8691	15573	3.09%	0.350%
7	3.841	858	871	875	rBV2	25398	55134	10.93%	1.240%
8	4.262	986	1002	1019	rBV3	89774	230578	45.71%	5.185%
9	4.516	1074	1081	1082	rBV6	4819	5066	1.00%	0.114%
10	4.966	1205	1221	1246	rBV2	193055	504403	100.00%	11.342%
11	5.542	1387	1400	1418	rBV	142422	299754	59.43%	6.740%
12	5.841	1476	1493	1514	rBV2	113999	237701	47.13%	5.345%
13	5.998	1529	1542	1561	rBV2	117493	245624	48.70%	5.523%
14	6.924	1817	1830	1850	rBV	50720	103673	20.55%	2.331%
15	7.252	1920	1932	1946	rBV	222385	397165	78.74%	8.931%
16	7.326	1947	1955	1974	rVB	37503	74913	14.85%	1.684%
17	7.564	2020	2029	2048	rBV3	30266	59201	11.74%	1.331%
18	7.911	2127	2137	2148	rBV3	47152	80823	16.02%	1.817%
19	8.040	2167	2177	2202	rBV	162110	381325	75.60%	8.574%
20	8.792	2400	2411	2431	rBV	215025	378578	75.05%	8.513%
21	9.767	2704	2714	2724	rBV	5913	11909	2.36%	0.268%
22	10.162	2825	2837	2850	rBV	83740	137963	27.35%	3.102%
23	10.995	3088	3096	3108	rBV2	15392	26421	5.24%	0.594%
24	11.194	3146	3158	3177	rVB	222454	357797	70.93%	8.045%
25	11.567	3260	3274	3291	rBV	219550	353140	70.01%	7.941%




Sum of corrected areas: 4447233

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042823\
Data File : VV030930.D
Acq On : 28 Apr 2023 18:57
Operator : SY/MD
Sample : 02488-19DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHE74DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

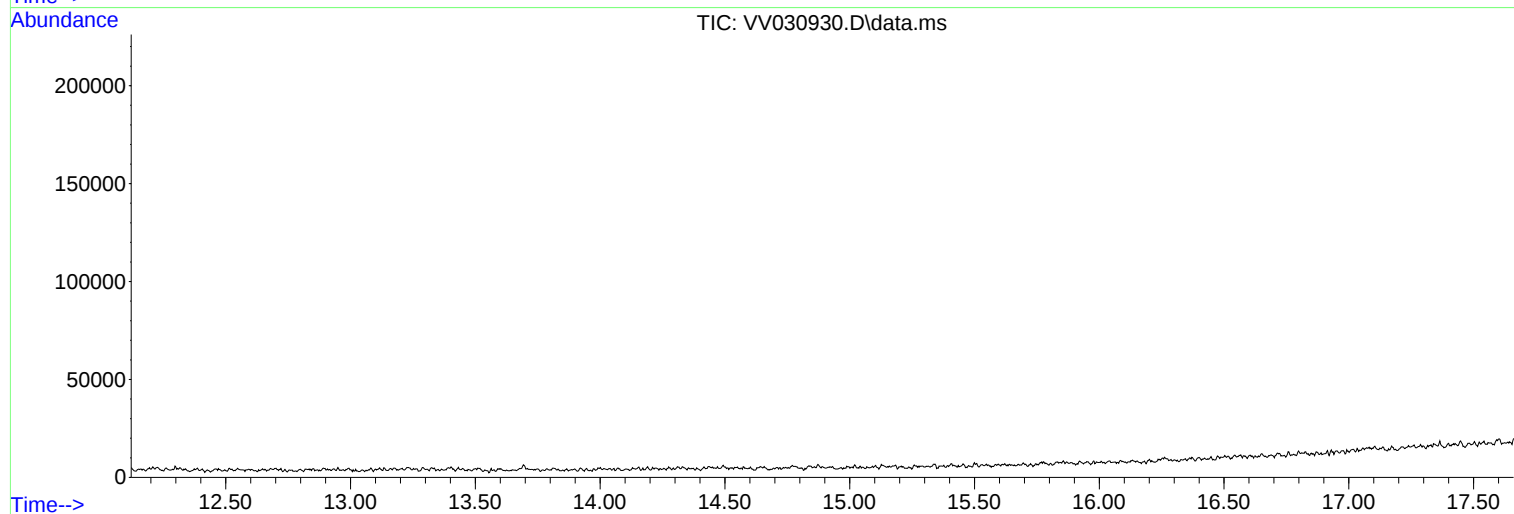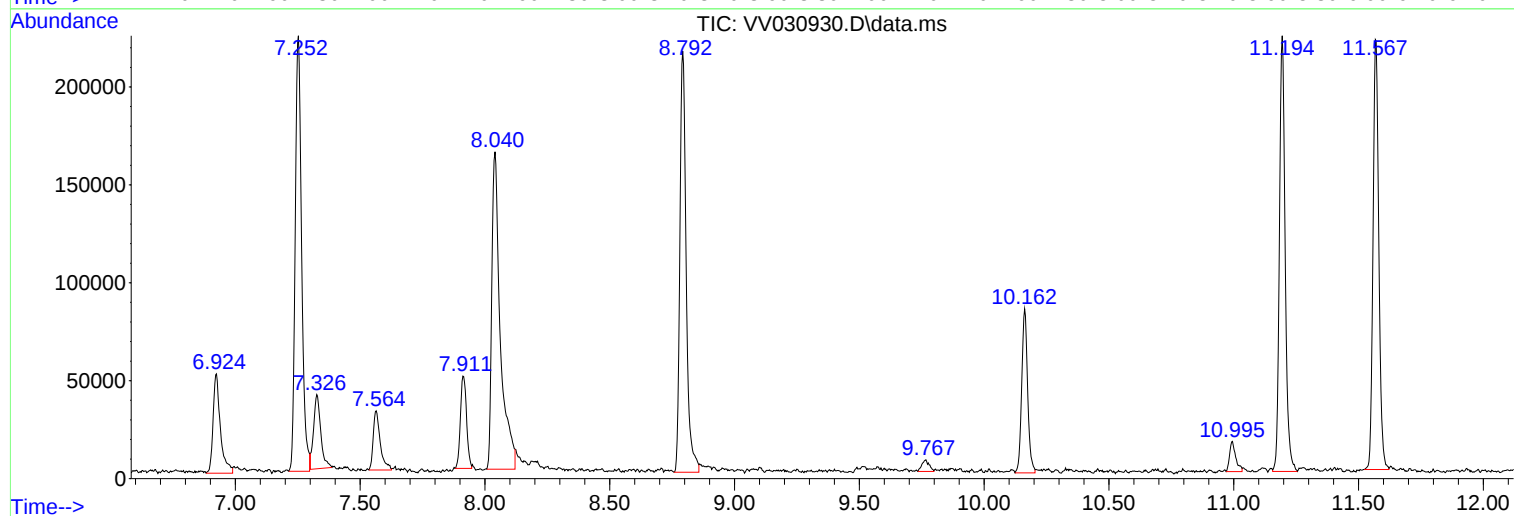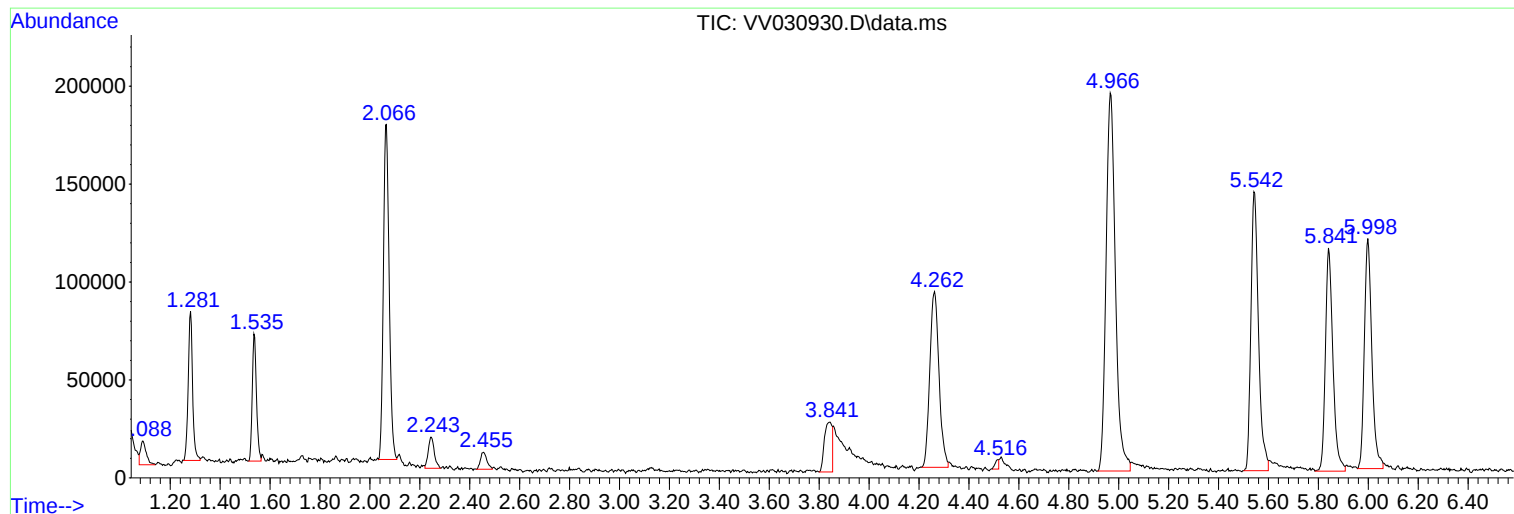

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042823\
Data File : VV030930.D
Acq On : 28 Apr 2023 18:57
Operator : SY/MD
Sample : 02488-19DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHE74DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042823\
Data File : VV030930.D
Acq On : 28 Apr 2023 18:57
Operator : SY/MD
Sample : 02488-19DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHE74DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc