

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042823\
 Data File : VV030931.D
 Acq On : 28 Apr 2023 19:22
 Operator : SY/MD
 Sample : 02488-20DL 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHE75DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030931.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	89	rVB	70719	83713	11.44%	1.632%
2	1.539	147	155	166	rVB	66805	77234	10.56%	1.506%
3	2.072	307	321	344	rBV5	440954	731632	100.00%	14.263%
4	2.455	430	440	453	rVB3	11782	21426	2.93%	0.418%
5	3.121	634	647	659	rBV2	19682	43003	5.88%	0.838%
6	3.821	855	865	891	rBV	42386	149154	20.39%	2.908%
7	4.262	983	1002	1022	rBV2	98911	246051	33.63%	4.797%
8	4.522	1065	1083	1104	rVB3	51160	136859	18.71%	2.668%
9	4.966	1204	1221	1242	rBV2	190102	488835	66.81%	9.530%
10	5.545	1387	1401	1422	rBV	142907	308987	42.23%	6.024%
11	5.847	1485	1495	1504	rBV	8668	18466	2.52%	0.360%
12	5.998	1529	1542	1565	rBV	113778	239659	32.76%	4.672%
13	6.921	1817	1829	1846	rBV3	47718	95680	13.08%	1.865%
14	7.252	1920	1932	1950	rBV	212167	380990	52.07%	7.427%
15	7.564	2020	2029	2046	rBV2	28637	54102	7.39%	1.055%
16	7.911	2123	2137	2156	rBV	280506	483045	66.02%	9.417%
17	8.037	2166	2176	2209	rBV	169526	376068	51.40%	7.331%
18	8.792	2400	2411	2436	rBV	218975	371753	50.81%	7.247%
19	10.162	2826	2837	2858	rVB2	79439	134401	18.37%	2.620%
20	11.194	3144	3158	3173	rBV	212002	349915	47.83%	6.822%
21	11.570	3264	3275	3291	rBV	207026	338568	46.28%	6.600%




Sum of corrected areas: 5129541

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042823\
Data File : VV030931.D
Acq On : 28 Apr 2023 19:22
Operator : SY/MD
Sample : 02488-20DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHE75DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

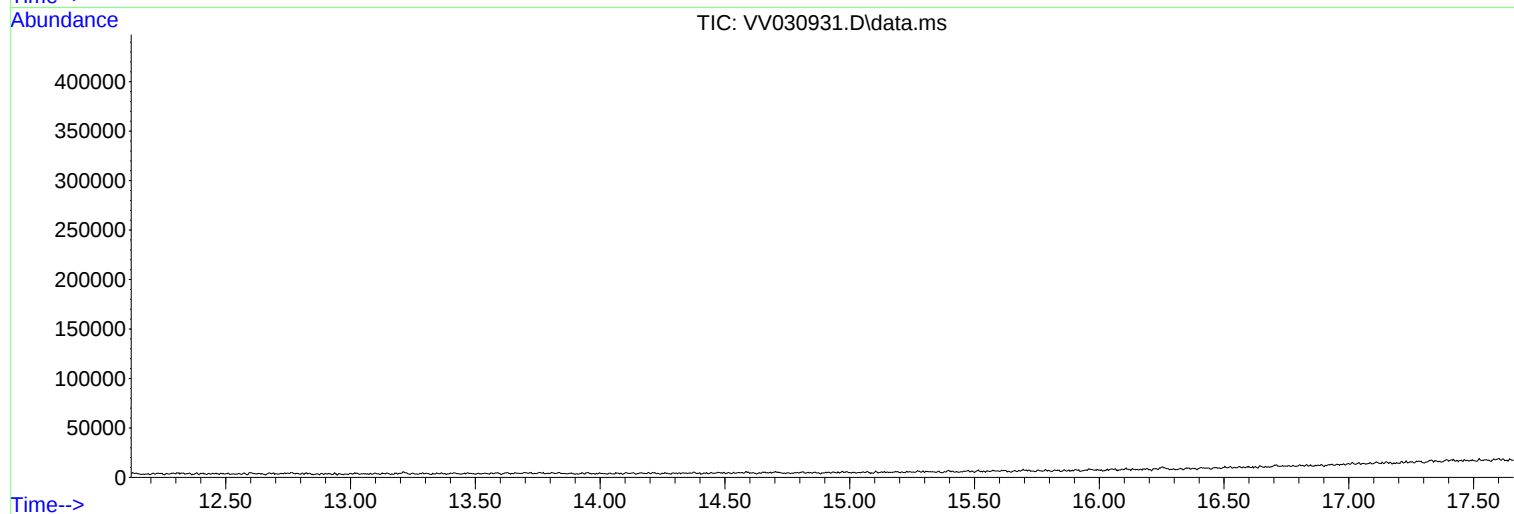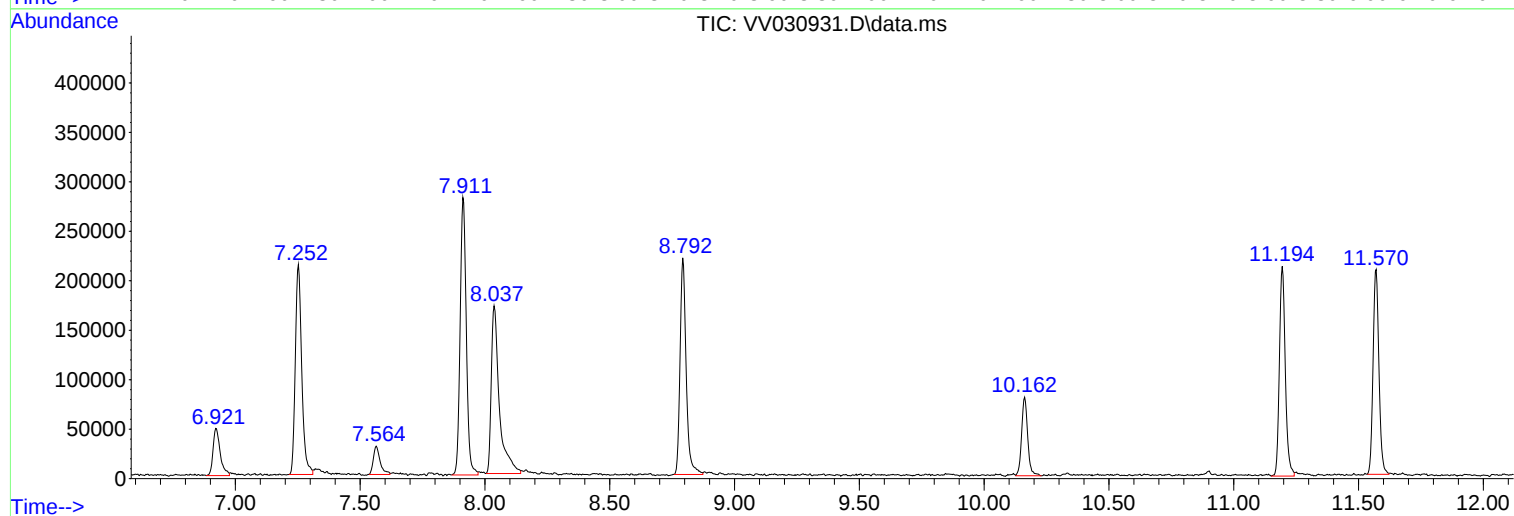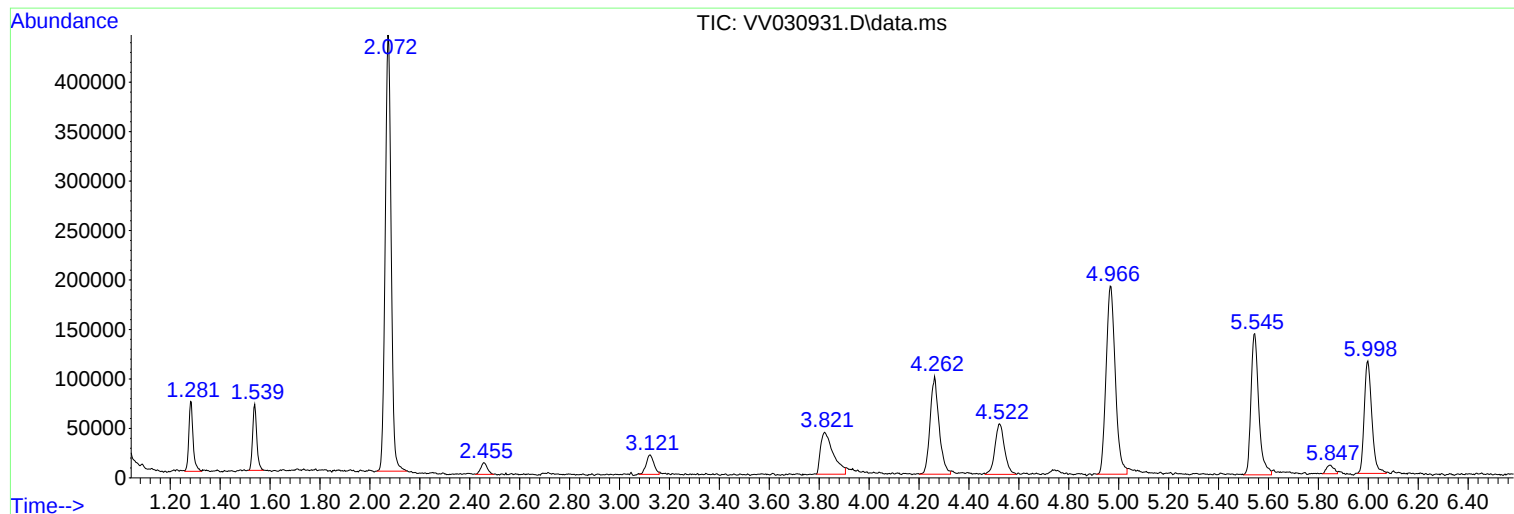

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042823\
Data File : VV030931.D
Acq On : 28 Apr 2023 19:22
Operator : SY/MD
Sample : 02488-20DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHE75DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042823\
Data File : VV030931.D
Acq On : 28 Apr 2023 19:22
Operator : SY/MD
Sample : 02488-20DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHE75DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc