

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042823\
 Data File : VV030935.D
 Acq On : 28 Apr 2023 21:00
 Operator : SY/MD
 Sample : 02488-20
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHE75

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030935.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	67	75	86	rBV2	86237	102798	1.83%	0.603%
2	1.539	146	155	166	rVB	65644	79891	1.42%	0.469%
3	2.076	307	322	355	rBV	3808367	5628076	100.00%	33.024%
4	3.121	629	647	665	rBV	192858	413307	7.34%	2.425%
5	3.822	851	865	891	rBV3	92462	285307	5.07%	1.674%
6	4.262	983	1002	1028	rBV4	103519	326850	5.81%	1.918%
7	4.522	1065	1083	1112	rBV	506991	1294929	23.01%	7.598%
8	4.748	1139	1153	1170	rVB2	45039	109237	1.94%	0.641%
9	4.966	1204	1221	1242	rBV2	196414	523154	9.30%	3.070%
10	5.542	1388	1400	1418	rBV	147302	311691	5.54%	1.829%
11	5.841	1478	1493	1509	rBV2	71323	153162	2.72%	0.899%
12	5.998	1527	1542	1561	rBV2	117676	247569	4.40%	1.453%
13	6.921	1814	1829	1850	rBV2	49353	103654	1.84%	0.608%
14	7.252	1919	1932	1947	rBV	220660	395652	7.03%	2.322%
15	7.561	2018	2028	2046	rBV2	31087	61454	1.09%	0.361%
16	7.911	2122	2137	2165	rBV	3206223	5327306	94.66%	31.259%
17	8.037	2165	2176	2208	rVB	198349	425370	7.56%	2.496%
18	8.792	2398	2411	2433	rBV	226848	397972	7.07%	2.335%
19	10.162	2827	2837	2851	rVB2	83915	135007	2.40%	0.792%
20	11.194	3147	3158	3173	rBV	223998	363406	6.46%	2.132%
21	11.570	3263	3275	3293	rVB	216377	356461	6.33%	2.092%




Sum of corrected areas: 17042253

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042823\
Data File : VV030935.D
Acq On : 28 Apr 2023 21:00
Operator : SY/MD
Sample : 02488-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHE75

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

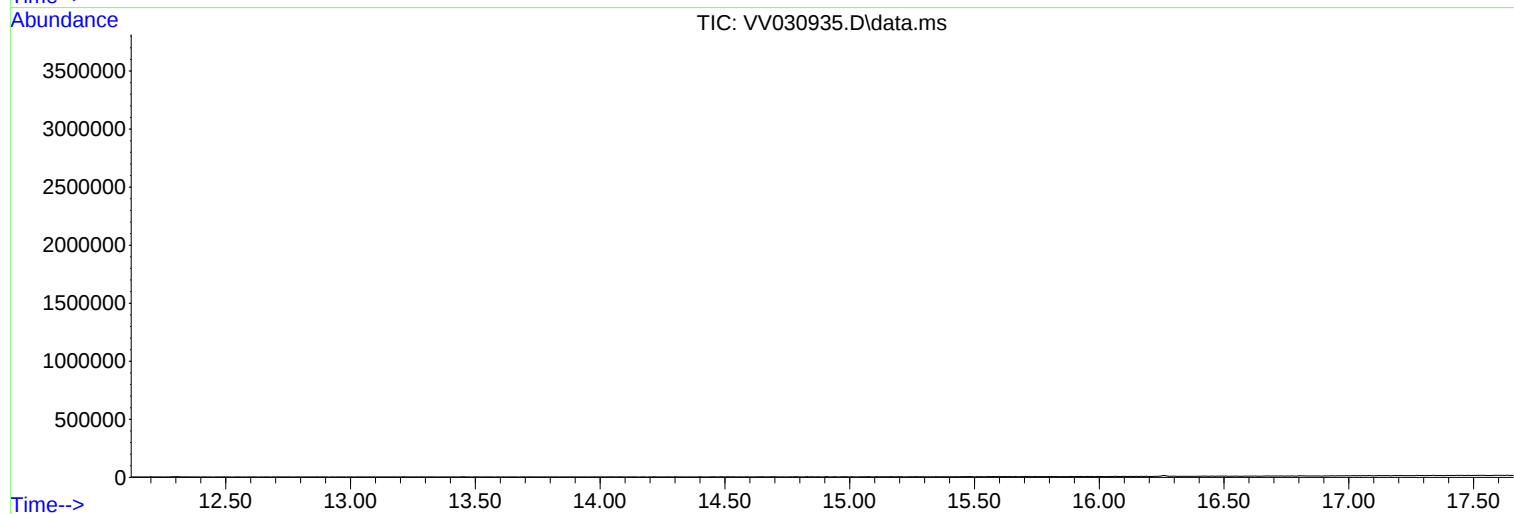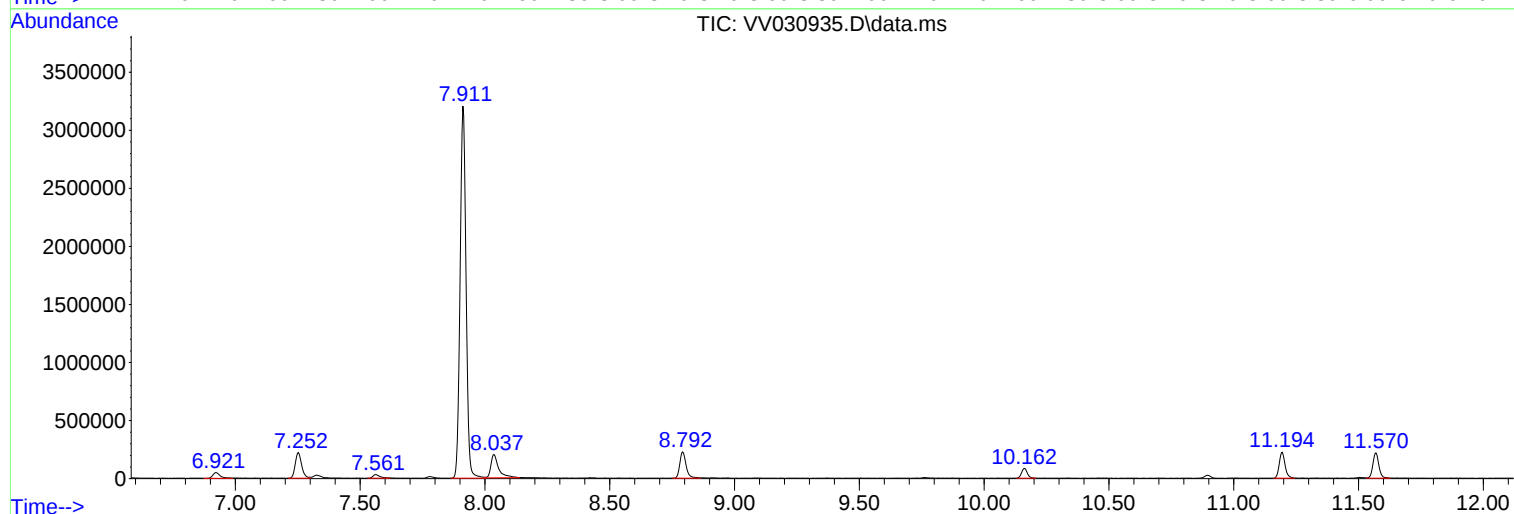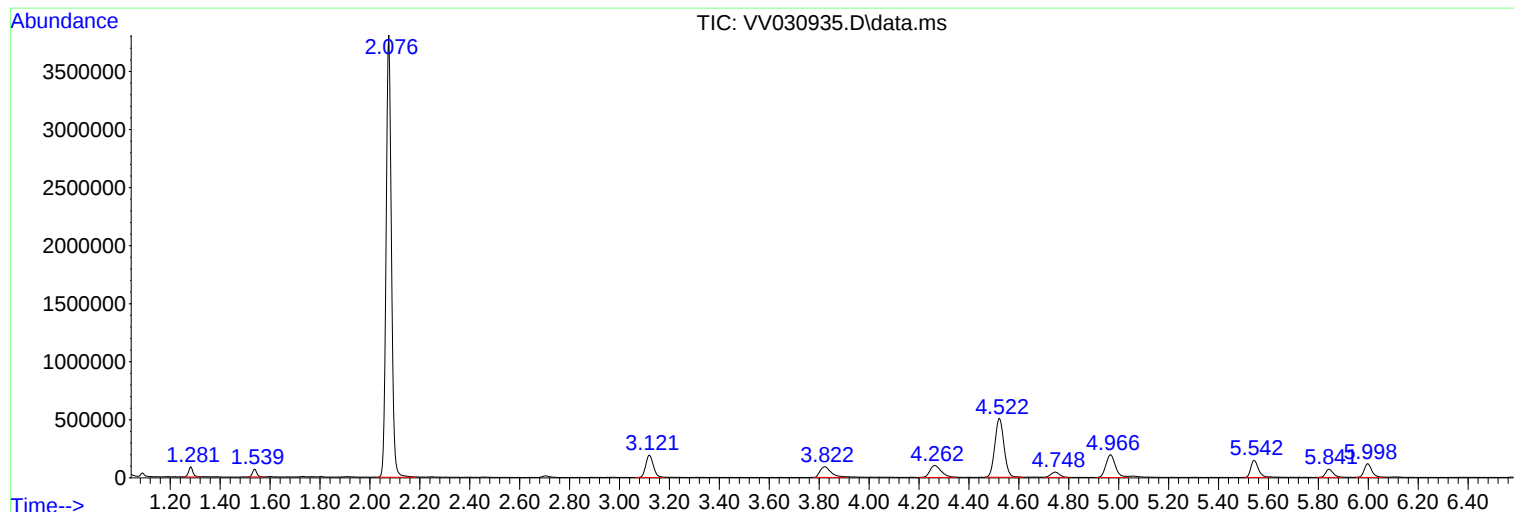

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042823\
Data File : VV030935.D
Acq On : 28 Apr 2023 21:00
Operator : SY/MD
Sample : 02488-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHE75

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042823\
Data File : VV030935.D
Acq On : 28 Apr 2023 21:00
Operator : SY/MD
Sample : 02488-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHE75

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
