

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042823\
 Data File : VV030937.D
 Acq On : 28 Apr 2023 21:50
 Operator : SY/MD
 Sample : 02551-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHE78

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030937.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.285	67	76	86	rBV	75067	85475	15.85%	2.032%
2	1.539	147	155	167	rBV	74816	85686	15.89%	2.037%
3	2.066	307	319	330	rBV	148421	219589	40.72%	5.221%
4	3.815	849	863	888	rBV2	46392	160251	29.72%	3.810%
5	4.259	984	1001	1021	rBV2	101646	265560	49.24%	6.314%
6	4.966	1204	1221	1247	rBV3	206548	539284	100.00%	12.823%
7	5.542	1388	1400	1421	rBV	139585	297255	55.12%	7.068%
8	5.998	1528	1542	1561	rBV2	125702	265391	49.21%	6.310%
9	6.921	1819	1829	1845	rBV3	51185	102153	18.94%	2.429%
10	7.252	1920	1932	1949	rBV	231505	412330	76.46%	9.804%
11	7.561	2020	2028	2044	rBV	32505	61073	11.32%	1.452%
12	7.915	2133	2138	2149	rVB10	4024	5961	1.11%	0.142%
13	8.037	2160	2176	2208	rBV	188389	425883	78.97%	10.126%
14	8.792	2399	2411	2431	rBV	220430	377460	69.99%	8.975%
15	10.162	2826	2837	2853	rVB	86734	143241	26.56%	3.406%
16	10.333	2883	2890	2901	rVB8	5061	8831	1.64%	0.210%
17	11.191	3145	3157	3179	rBV	212260	347450	64.43%	8.261%
18	11.567	3261	3274	3290	rVV	231109	372707	69.11%	8.862%
19	12.297	3492	3501	3511	rBV9	17436	30094	5.58%	0.716%




Sum of corrected areas: 4205674

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042823\
Data File : VV030937.D
Acq On : 28 Apr 2023 21:50
Operator : SY/MD
Sample : 02551-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHE78

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

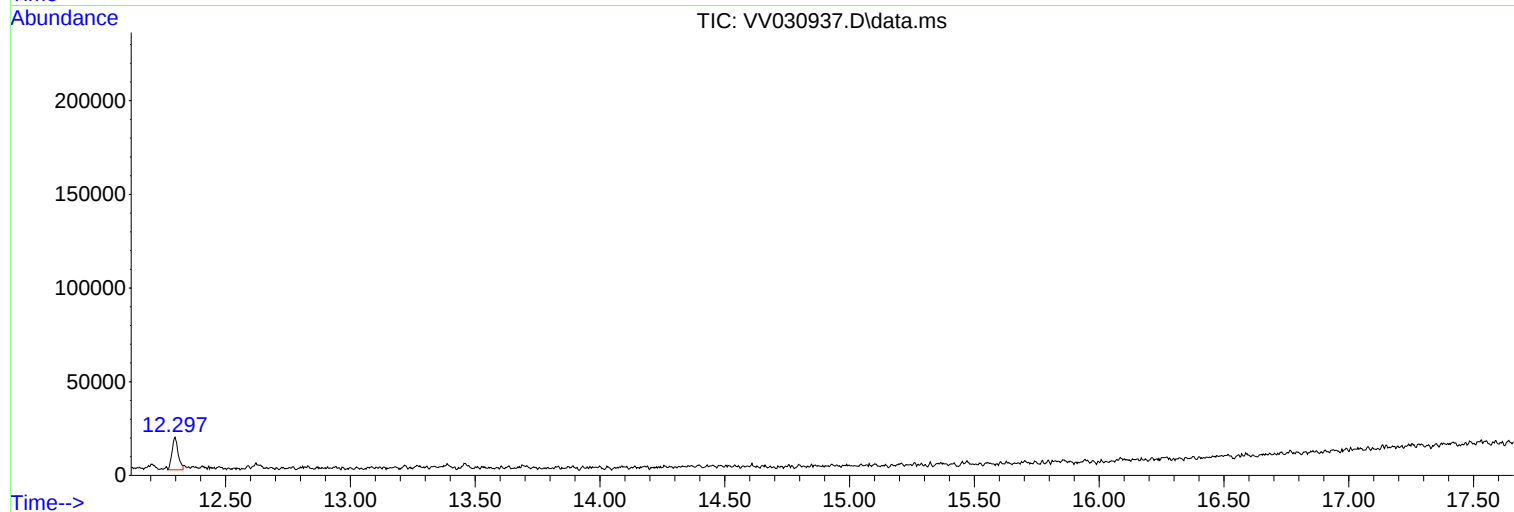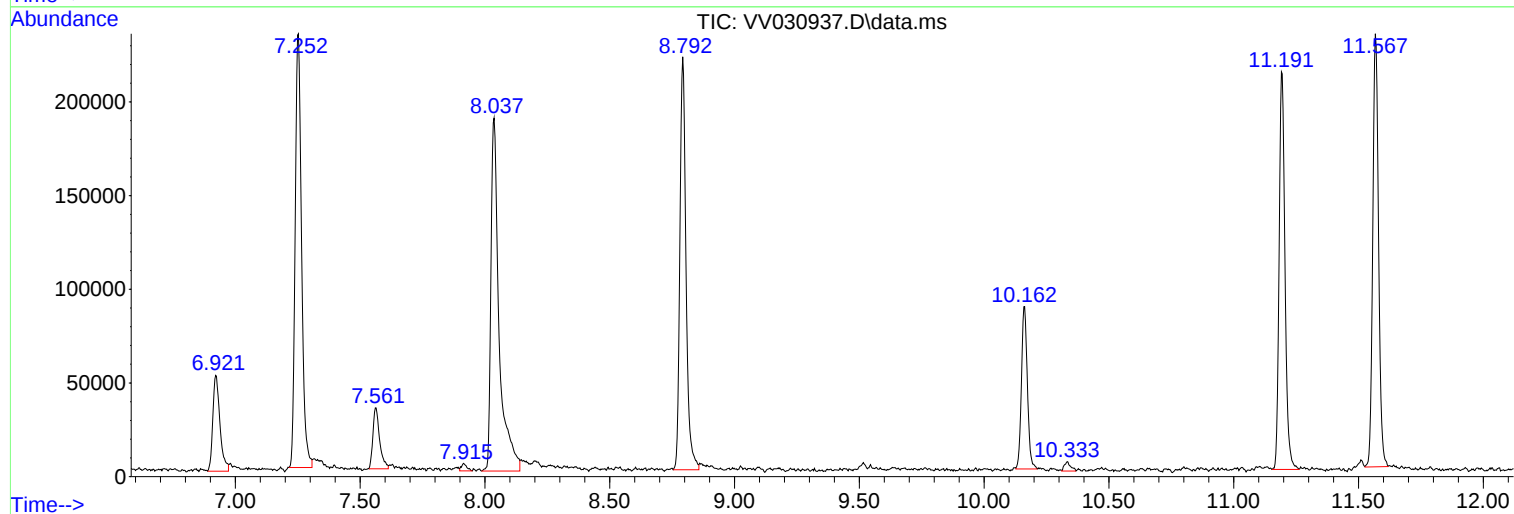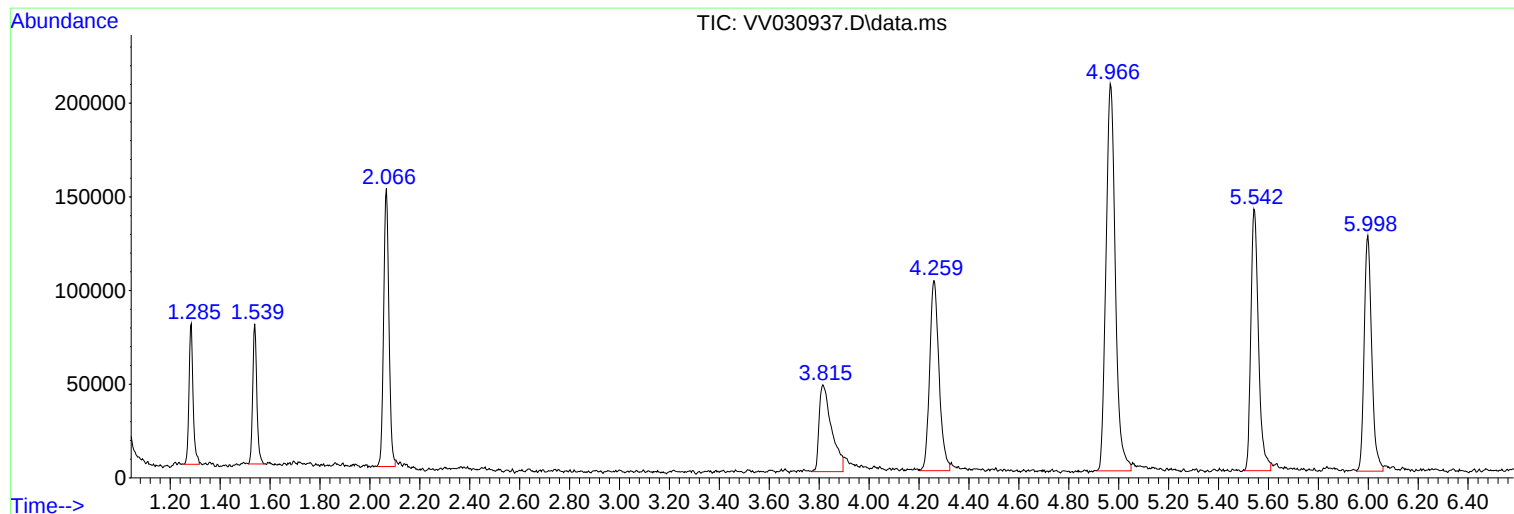

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042823\
Data File : VV030937.D
Acq On : 28 Apr 2023 21:50
Operator : SY/MD
Sample : 02551-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHE78

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042823\
Data File : VV030937.D
Acq On : 28 Apr 2023 21:50
Operator : SY/MD
Sample : 02551-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHE78

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc