
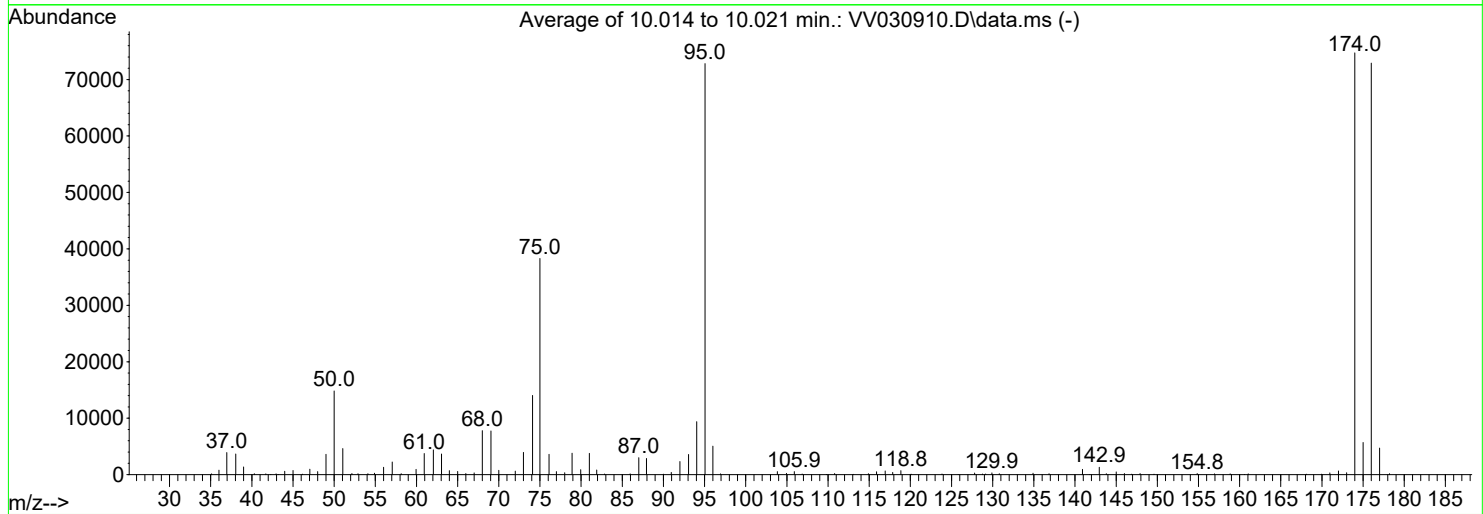


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042823\
 Data File : VV030910.D
 Acq On : 28 Apr 2023 08:51
 Operator : SY/MD
 Sample : BFB255
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB255

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Sat Apr 29 01:06:38 2023

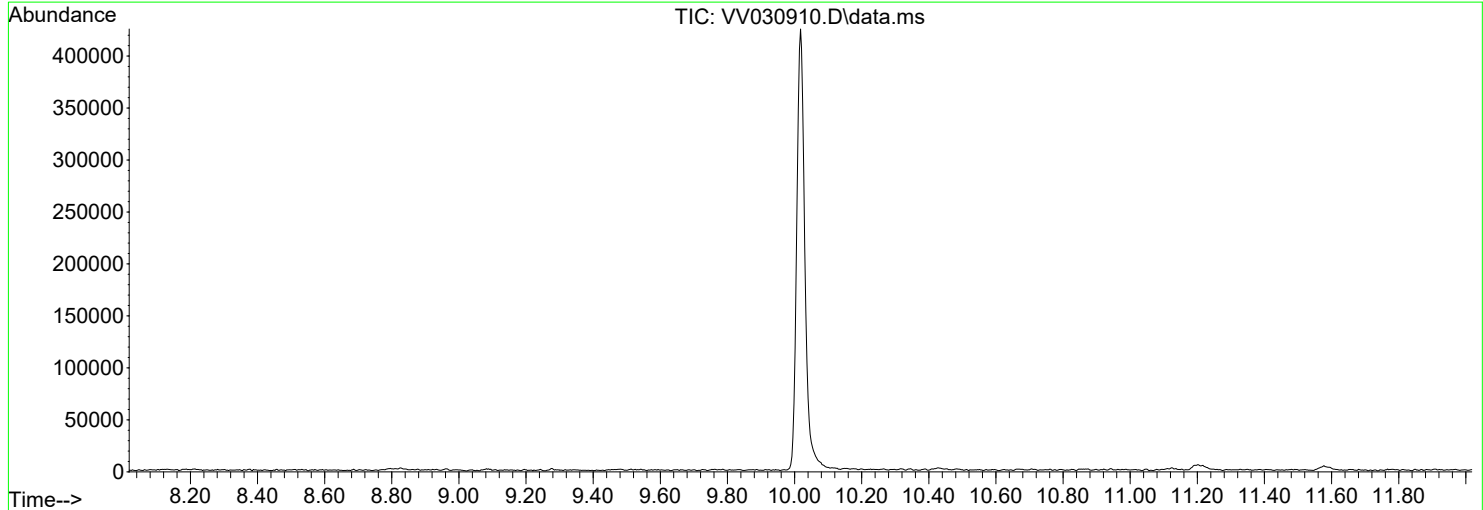

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	14830	PASS
75	95	30	80	52.6	38309	PASS
95	95	100	100	100.0	72816	PASS
96	95	5	9	6.9	5054	PASS
173	174	0.00	2	0.5	347	PASS
174	95	50	120	102.6	74731	PASS
175	174	5	9	7.6	5701	PASS
176	174	95	105	97.6	72912	PASS
177	176	5	10	6.5	4706	PASS

m/z	Abundance
35.70	131.0
36.90	169.0
37.60	132.0
39.00	141.0
40.00	186.0
41.20	127.0
44.00	240.0
45.20	111.0
45.70	108.0
50.40	141.0
52.60	101.0
57.60	113.0
60.90	118.0
69.40	116.0

Instrument :
MSVOA_V
ClientSampleId :
BFB255

m/z	Abundance
35.10	136.0
36.00	768.0
37.00	3983.0
38.00	3696.0
39.00	1529.0
40.10	268.0
41.70	139.0
42.90	130.0
43.20	121.0
44.00	867.0
45.00	831.0
47.10	1055.0
48.00	577.0
49.00	3609.0
50.00	14574.0
51.00	4711.0
52.10	186.0
52.80	151.0
54.10	149.0
54.90	238.0
56.00	1336.0
57.00	2171.0
58.10	174.0
59.90	985.0
61.00	3937.0
62.10	4394.0
63.00	3518.0
64.00	742.0
65.00	532.0
66.00	181.0
67.00	307.0
68.00	7626.0
69.00	7572.0
70.00	690.0
72.00	560.0
73.00	3888.0
74.10	13753.0
75.00	38384.0
76.10	3629.0
77.00	582.0
78.00	303.0
78.90	3829.0
79.90	850.0
81.00	3764.0
81.90	824.0
82.80	112.0
86.00	141.0
87.00	3002.0
88.00	3047.0
90.00	118.0
91.00	382.0
92.00	2238.0
93.10	3465.0
94.00	9243.0
95.10	71808.0
96.00	4974.0
96.90	113.0
103.90	467.0
104.90	201.0
105.90	512.0
106.90	119.0
109.80	116.0
110.80	181.0
114.90	163.0
115.90	457.0
116.90	625.0
117.80	413.0
118.90	761.0
123.90	130.0
127.80	310.0
128.70	108.0
129.10	105.0
129.90	280.0
130.80	184.0
134.90	273.0
136.90	165.0
140.90	916.0
141.80	125.0
142.90	1288.0
143.80	143.0
145.00	472.0
146.00	218.0
146.90	143.0
147.80	214.0
155.00	187.0
157.00	176.0
158.90	145.0
161.10	100.0
168.10	130.0
171.10	337.0
172.00	600.0
173.00	1042.0

Instrument :
MSVOA_V
ClientSampleId :
BFB255

174.00	71928.0
175.00	5426.0
176.00	70776.0
177.00	4743.0
178.20	176.0

Instrument :
MSVOA_V
ClientSampleId :
BFB255

m/z	Abundance
35.10	163.0
36.00	811.0
37.00	4228.0
38.00	3693.0
39.00	1537.0
40.30	290.0
41.70	147.0
42.90	156.0
44.00	878.0
45.00	886.0
46.20	142.0
47.10	991.0
48.00	537.0
49.00	3778.0
50.00	15347.0
51.00	4700.0
52.20	214.0
52.90	166.0
54.10	185.0
54.90	253.0
56.00	1367.0
57.10	2324.0
58.20	177.0
60.00	952.0
61.00	3987.0
62.00	4494.0
63.10	3785.0
64.00	732.0
65.00	575.0
66.00	201.0
67.00	329.0
68.00	8037.0
69.10	7946.0
70.00	816.0
72.00	670.0
73.00	4097.0
74.10	14425.0
75.00	39520.0
76.10	3753.0
77.00	552.0
78.00	369.0
78.90	3898.0
79.90	908.0
81.00	3849.0
81.90	841.0
82.90	131.0
85.90	152.0
87.00	3074.0
88.00	2931.0
90.00	122.0
90.90	400.0
92.00	2379.0
93.10	3677.0
94.10	9663.0
95.00	75096.0
96.00	5235.0
97.00	147.0
103.80	561.0
105.00	244.0
105.90	570.0
106.90	122.0
110.80	211.0
113.00	104.0
114.90	165.0
115.90	554.0
117.00	654.0
117.80	408.0
118.80	702.0
120.10	112.0
123.90	142.0
127.80	274.0
128.80	110.0
129.10	112.0
129.90	333.0
130.80	182.0
134.90	250.0
136.90	171.0
140.90	988.0
142.90	1306.0
143.80	197.0
145.00	502.0
146.00	189.0
146.90	118.0
147.90	196.0
149.60	135.0
154.80	198.0
157.00	159.0
158.90	158.0
161.00	145.0
168.10	101.0
169.90	110.0
170.90	322.0

Instrument :
MSVOA_V
ClientSampleId :
BFB255

172.00	660.0
174.00	77120.0
175.00	5862.0
176.00	75728.0
177.00	4906.0
178.20	176.0

Instrument :
MSVOA_V
ClientSampleId :
BFB255

m/z	Abundance
35.10	159.0
36.00	784.0
37.00	4032.0
38.10	3596.0
39.10	1468.0
40.30	257.0
41.70	121.0
42.30	115.0
43.00	170.0
44.00	800.0
45.00	854.0
46.10	161.0
47.00	853.0
48.00	518.0
49.00	3412.0
50.00	14570.0
51.10	4429.0
52.10	226.0
53.00	209.0
54.10	188.0
54.90	245.0
56.00	1178.0
57.10	2254.0
58.10	156.0
60.00	899.0
61.00	3642.0
62.00	4273.0
63.10	3667.0
64.00	694.0
65.00	610.0
66.00	212.0
67.00	316.0
68.00	7733.0
69.10	7666.0
70.00	781.0
72.00	622.0
73.00	3866.0
74.10	13888.0
75.00	37024.0
76.10	3437.0
77.00	512.0
78.00	385.0
78.90	3718.0
80.00	902.0
81.00	3696.0
81.90	785.0
82.90	121.0
85.90	155.0
87.00	2954.0
87.90	2616.0
90.90	435.0
92.00	2342.0
93.00	3595.0
94.10	9245.0
95.00	71544.0
96.00	4952.0
97.00	199.0
103.80	590.0
105.00	255.0
105.90	553.0
106.80	145.0
110.80	206.0
113.10	104.0
114.90	197.0
115.90	506.0
117.00	671.0
117.90	399.0
118.90	630.0
120.10	119.0
123.80	120.0
125.80	126.0
127.80	274.0
128.80	118.0
129.20	132.0
129.90	346.0
130.80	137.0
134.90	246.0
136.80	168.0
140.90	948.0
143.00	1364.0
143.80	194.0
145.00	474.0
146.00	156.0
148.00	183.0
149.60	147.0
154.80	217.0
156.90	133.0
158.80	157.0
160.60	111.0
161.00	154.0
170.00	106.0
170.80	300.0

Instrument :
MSVOA_V
ClientSampleId :
BFB255

172.00	693.0
174.00	75144.0
175.00	5814.0
176.00	72232.0
177.00	4470.0
178.20	144.0

Instrument :
MSVOA_V
ClientSampleId :
BFB255