


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042919\
 Data File : VV010541.D
 Acq On : 29 Apr 2019 10:41
 Operator : SY/MD
 Sample : BFB04
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB04

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042619SIM.M
 Title : TRACE VOA SOM01.0
 Last Update : Tue Apr 30 01:23:26 2019

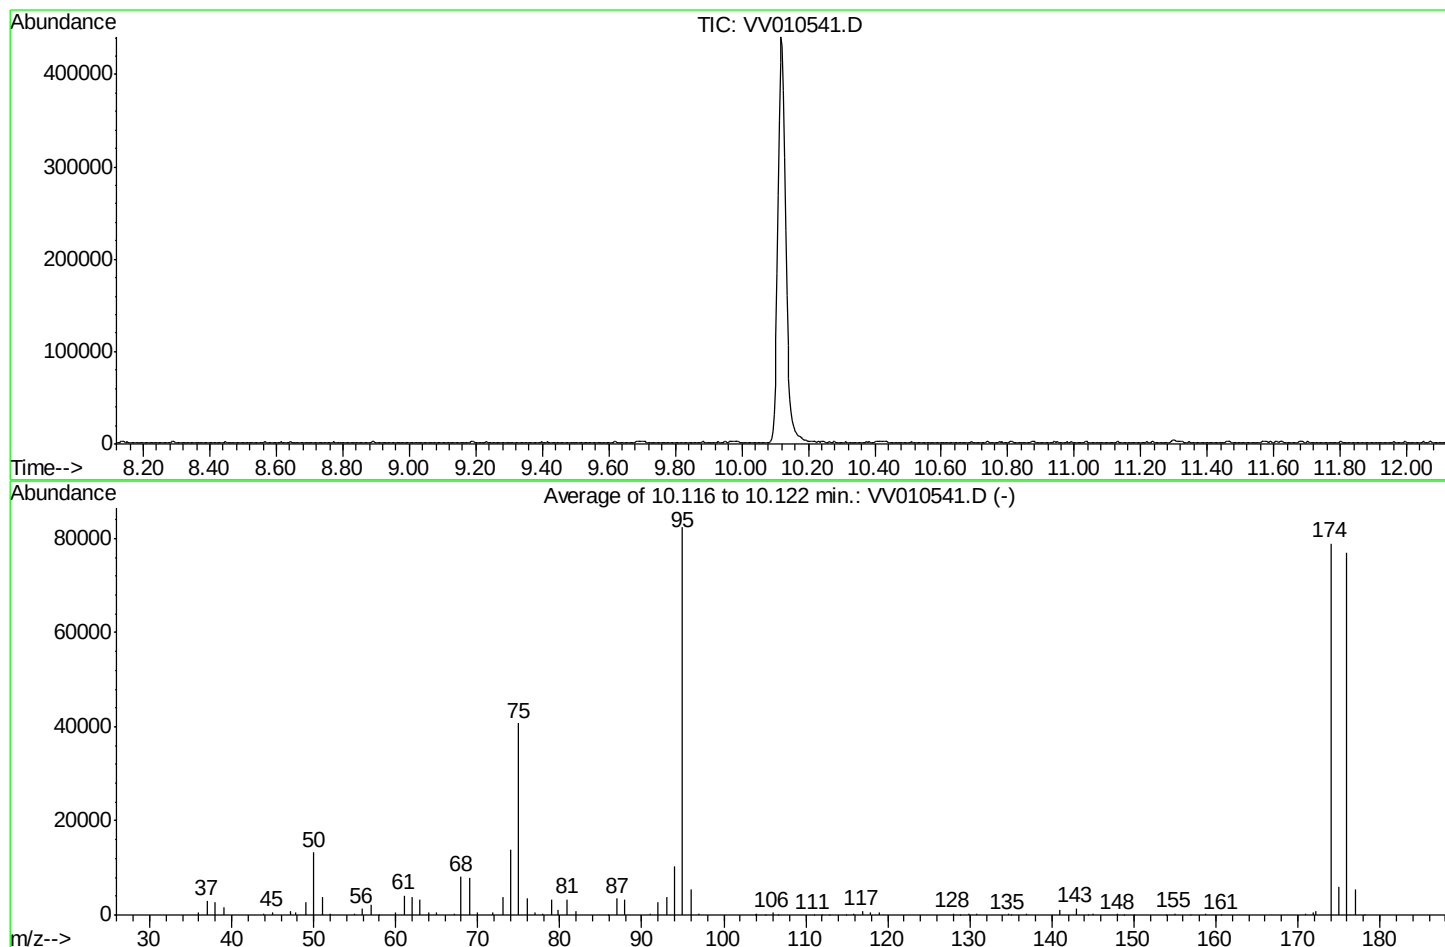

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	13324	PASS
75	95	30	80	49.5	40784	PASS
95	95	100	100	100.0	82362	PASS
96	95	5	9	6.7	5490	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	95.9	78954	PASS
175	174	5	9	7.5	5952	PASS
176	174	95	101	97.5	76970	PASS
177	176	5	9	6.9	5333	PASS

Scan 2794 (10.074 min): VV010541.D
BFB04

m/z	Abundance
39.90	1723.0
44.00	326.0

Instrument :
MSVOA_V
ClientSampleId :
BFB04

m/z	Abundance
35.90	612.0
37.00	3039.0
38.00	2736.0
39.00	1437.0
40.00	1526.0
43.90	715.0
45.00	593.0
47.10	794.0
47.90	334.0
49.00	2722.0
50.00	13143.0
51.00	3708.0
51.90	234.0
55.00	317.0
55.90	1190.0
57.00	2069.0
57.90	112.0
59.90	515.0
61.00	3959.0
62.00	3998.0
63.00	3229.0
64.10	622.0
65.00	594.0
67.10	155.0
68.00	7990.0
69.00	7509.0
70.00	479.0
71.90	409.0
73.00	3701.0
74.00	13329.0
75.00	39680.0
76.00	3574.0
76.90	547.0
77.90	256.0
78.90	3279.0
79.90	936.0
81.00	3277.0
81.90	908.0
85.80	144.0
87.00	3367.0
87.90	3062.0
91.00	312.0
91.90	2332.0
93.00	3745.0
94.00	10156.0
95.00	80888.0
96.00	5467.0
97.00	151.0
103.80	337.0
104.00	331.0
106.00	453.0
106.60	102.0
111.10	124.0
112.90	114.0
115.80	306.0
116.80	786.0
117.80	443.0
118.90	562.0
127.90	282.0
128.80	101.0
130.00	323.0
130.80	211.0
134.60	211.0
135.00	161.0
136.90	193.0
141.00	1072.0
142.90	1350.0
145.10	323.0
148.10	234.0
148.80	107.0
155.00	237.0
158.70	124.0
160.70	130.0
171.00	140.0
172.10	1245.0
174.00	74808.0
175.00	5872.0
176.00	73008.0
177.00	4915.0
178.10	114.0

Instrument :
MSVOA_V
ClientSampleId :
BFB04

m/z	Abundance
36.00	676.0
37.00	3223.0
38.00	2916.0
39.00	1734.0
40.00	1699.0
43.90	681.0
45.00	608.0
47.10	872.0
47.80	457.0
49.00	2927.0
50.00	13620.0
51.00	3920.0
52.00	227.0
55.00	363.0
55.90	1304.0
57.00	2133.0
57.90	126.0
59.90	538.0
61.00	4165.0
62.00	4075.0
63.00	3440.0
64.10	532.0
65.00	677.0
67.10	231.0
68.00	8379.0
69.00	8102.0
70.00	570.0
71.90	455.0
73.00	3835.0
74.00	14278.0
75.00	42016.0
76.00	3798.0
76.90	599.0
77.80	372.0
79.00	3351.0
79.90	1072.0
80.90	3446.0
81.90	969.0
85.80	119.0
87.00	3596.0
87.90	3232.0
91.00	312.0
92.00	2836.0
93.00	3899.0
94.00	10693.0
95.00	84536.0
96.00	5750.0
96.90	206.0
104.00	377.0
106.00	539.0
106.60	106.0
111.00	151.0
113.00	125.0
114.90	130.0
115.80	439.0
116.90	802.0
117.90	480.0
118.90	722.0
128.00	398.0
128.70	114.0
130.00	347.0
130.80	200.0
134.70	261.0
136.90	186.0
141.00	1057.0
143.00	1448.0
144.40	137.0
145.00	307.0
148.00	267.0
153.90	103.0
154.90	291.0
156.90	113.0
158.70	153.0
160.70	150.0
171.00	212.0
172.10	1364.0
174.00	81496.0
175.00	6108.0
176.00	79064.0
177.00	5568.0

Instrument :
MSVOA_V
ClientSampleId :
BFB04

m/z	Abundance
36.00	680.0
37.00	2830.0
38.00	2784.0
39.10	1806.0
40.00	1807.0
43.90	768.0
44.90	588.0
47.10	712.0
47.80	482.0
49.00	2739.0
50.00	13210.0
51.00	3742.0
52.00	203.0
55.00	365.0
55.90	1215.0
57.00	2222.0
58.00	125.0
59.90	485.0
61.00	4153.0
62.00	3778.0
63.00	3374.0
64.00	474.0
65.00	741.0
67.10	239.0
68.00	7995.0
69.00	7913.0
70.00	616.0
71.90	427.0
73.00	3573.0
74.00	13689.0
75.00	40656.0
76.00	3591.0
76.90	532.0
77.80	402.0
79.00	3049.0
79.80	1149.0
80.90	3321.0
81.90	910.0
87.00	3265.0
87.90	3152.0
91.00	321.0
92.00	2878.0
93.00	3662.0
94.00	10419.0
95.00	81664.0
96.00	5254.0
96.90	211.0
104.00	401.0
105.10	152.0
106.00	483.0
110.90	130.0
111.90	106.0
112.90	117.0
114.90	179.0
115.80	457.0
117.00	887.0
117.80	483.0
119.00	760.0
128.00	470.0
128.80	140.0
129.90	348.0
130.80	171.0
134.70	322.0
136.90	192.0
141.00	1002.0
143.00	1516.0
144.40	162.0
145.00	271.0
148.00	226.0
150.00	131.0
153.90	116.0
154.90	335.0
156.90	153.0
158.70	184.0
160.70	124.0
171.00	236.0
171.80	1370.0
174.00	80560.0
175.10	5876.0
176.00	78840.0
177.00	5517.0

Instrument :
MSVOA_V
ClientSampleId :
BFB04