

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV042920\
 Data File : VV015783.D
 Acq On : 29 Apr 2020 11:31
 Operator : SY/MD
 Sample : VV0429WBL01
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK49

Quant Time: Apr 30 02:13:46 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Apr 30 01:35:08 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	131853	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	128037	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	59371	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	40242	5.84	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	116.80%
7) Chloroethane-d5	1.57	69	34887	5.25	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	105.00%
11) 1,1-Dichloroethene-d2	2.11	63	57852	3.84	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	76.80%
20) 2-Butanone-d5	3.95	46	98390	44.47	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	88.94%
24) Chloroform-d	4.37	84	68301	4.25	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.00%
26) 1,2-Dichloroethane-d4	5.06	65	43194	4.81	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.20%
32) Benzene-d6	5.07	84	143995	4.71	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.20%
36) 1,2-Dichloropropane-d6	6.09	67	44824	4.59	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	91.80%
41) Toluene-d8	7.34	98	125938	4.34	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.80%
43) trans-1,3-Dichloropropene-	7.65	79	14442	3.82	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	76.40%
46) 2-Hexanone-d5	8.12	63	67984	36.92	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	73.84%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	29349	4.04	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	80.80%
64) 1,2-Dichlorobenzene-d4	11.65	152	45113	4.47	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	89.40%


Target Compounds				Ovalue
25) Chloroform	4.40	83	7617	0.425 ug/L 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV042920\
Data File : VV015783.D
Acq On : 29 Apr 2020 11:31
Operator : SY/MD
Sample : VV0429WBL01
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK49

Quant Time: Apr 30 02:13:46 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Apr 30 01:35:08 2020
Response via : Initial Calibration

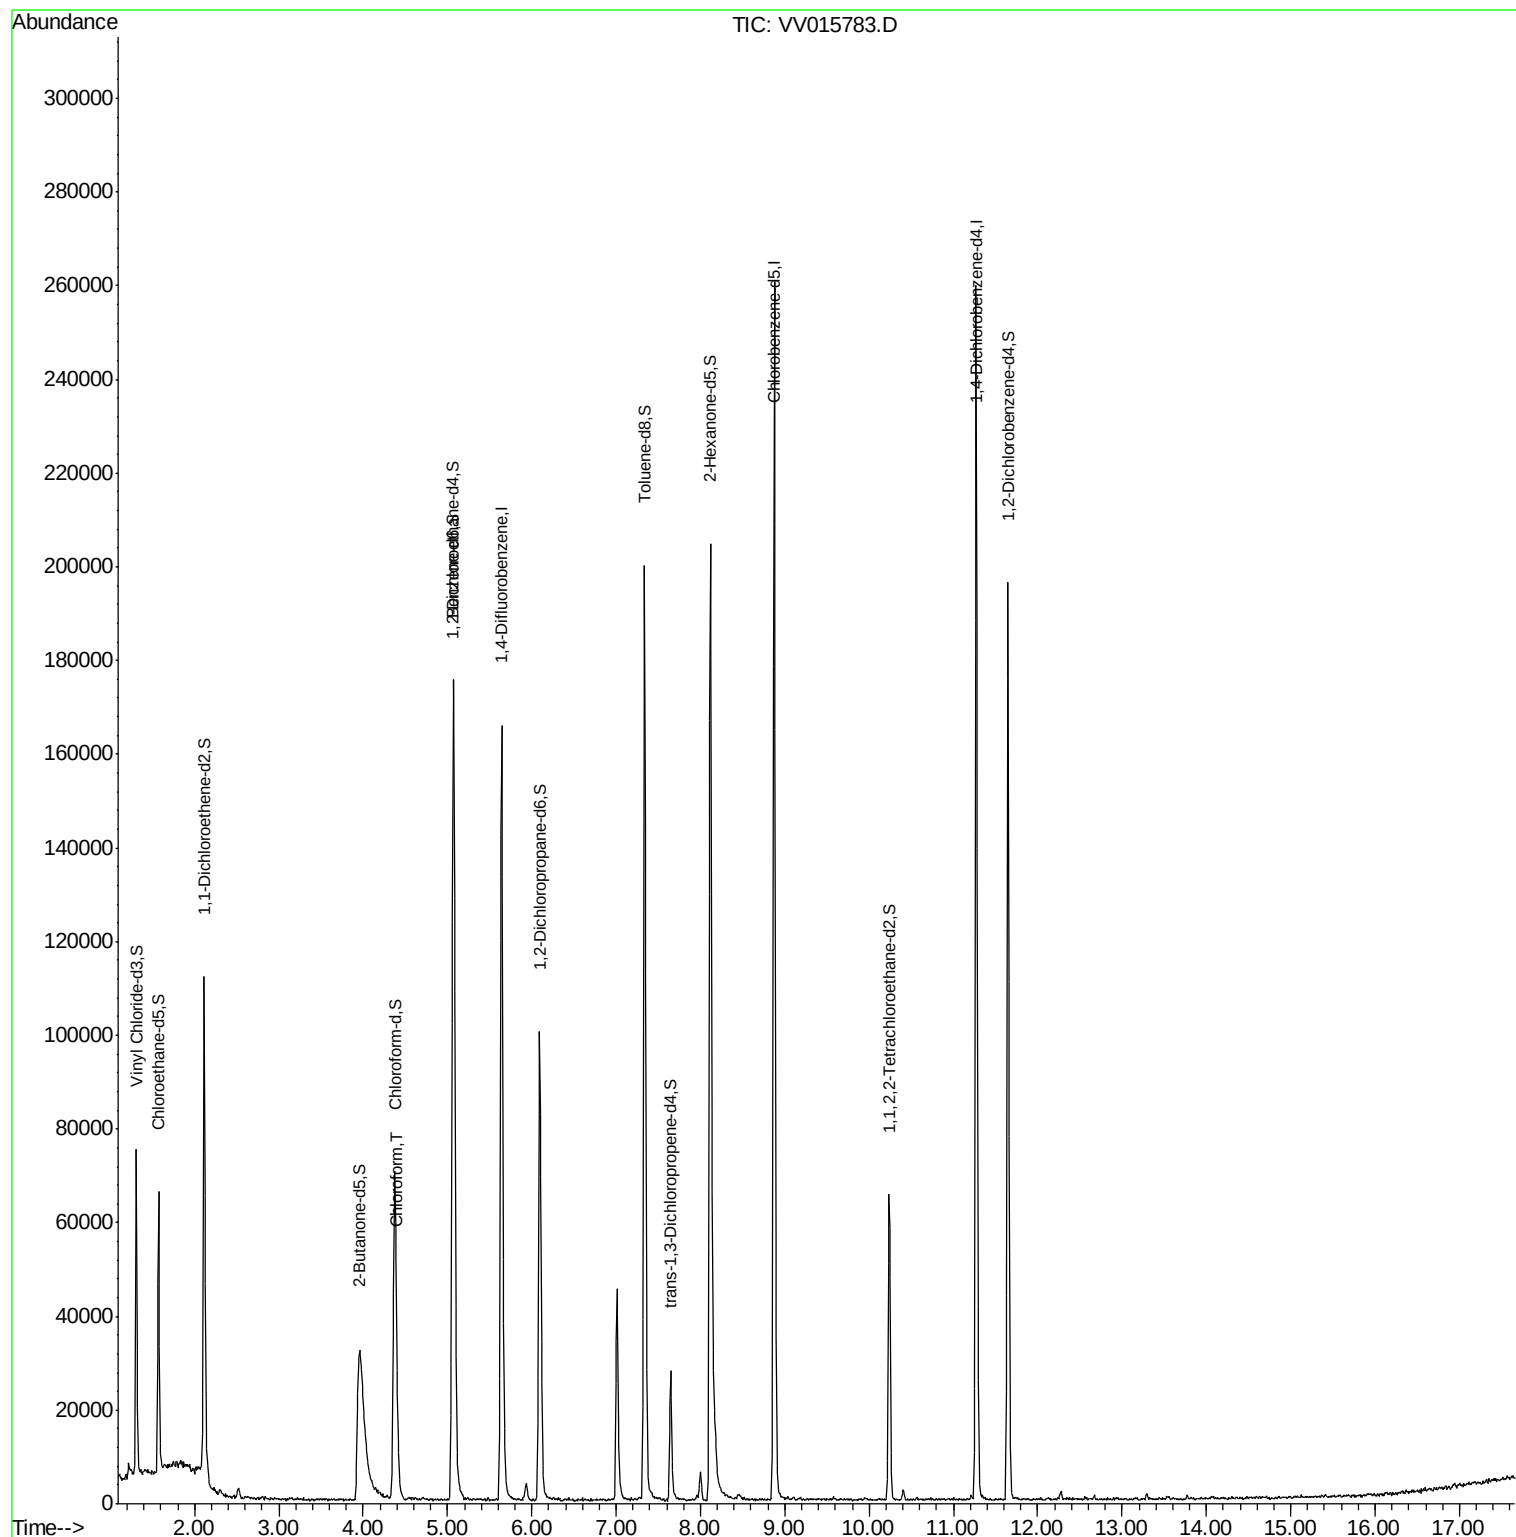

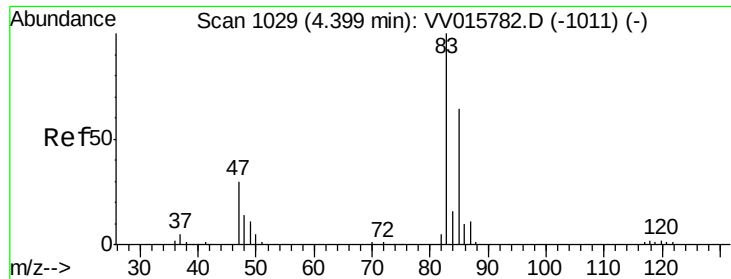

#25
 Chloroform
 Concen: 0.425 ug/L
 RT: 4.40 min Scan# 1030
 Delta R.T. 0.00 min
 Lab File: VV015783.D
 Acq: 29 Apr 2020 11:31

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK49

Tot Ion: 83 Resp: 7617
 Ion Ratio Lower Upper
 83 100
 85 60.3 46.1 85.5

