

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV042920\
 Data File : VV015810.D
 Acq On : 30 Apr 2020 00:06
 Operator : SY/MD
 Sample : L2431-04
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETKR3

Quant Time: Apr 30 07:44:58 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Apr 30 01:35:08 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	127647	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	122303	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	57635	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	37180	5.57	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	111.40%
7) Chloroethane-d5	1.58	69	33549	5.22	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	104.40%
11) 1,1-Dichloroethene-d2	2.12	63	53476	3.66	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.20%
20) 2-Butanone-d5	3.91	46	89247	41.67	ug/L	-0.04
Spiked Amount	50.000	Range	40 - 130	Recovery	=	83.34%
24) Chloroform-d	4.38	84	70088	4.51	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.20%
26) 1,2-Dichloroethane-d4	5.06	65	39782	4.57	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.40%
32) Benzene-d6	5.07	84	137556	4.71	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.20%
36) 1,2-Dichloropropane-d6	6.10	67	42302	4.53	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	90.60%
41) Toluene-d8	7.34	98	122455	4.42	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.40%
43) trans-1,3-Dichloropropene-	7.65	79	13562	3.76	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	75.20%
46) 2-Hexanone-d5	8.11	63	65164	37.05	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	74.10%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	28543	4.11	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	82.20%
64) 1,2-Dichlorobenzene-d4	11.65	152	44908	4.58	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	91.60%


Target Compounds					Ovalue
13) Acetone	2.18	43	2696	1.813 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV042920\
Data File : VV015810.D
Acq On : 30 Apr 2020 00:06
Operator : SY/MD
Sample : L2431-04
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETKR3

Quant Time: Apr 30 07:44:58 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Apr 30 01:35:08 2020
Response via : Initial Calibration

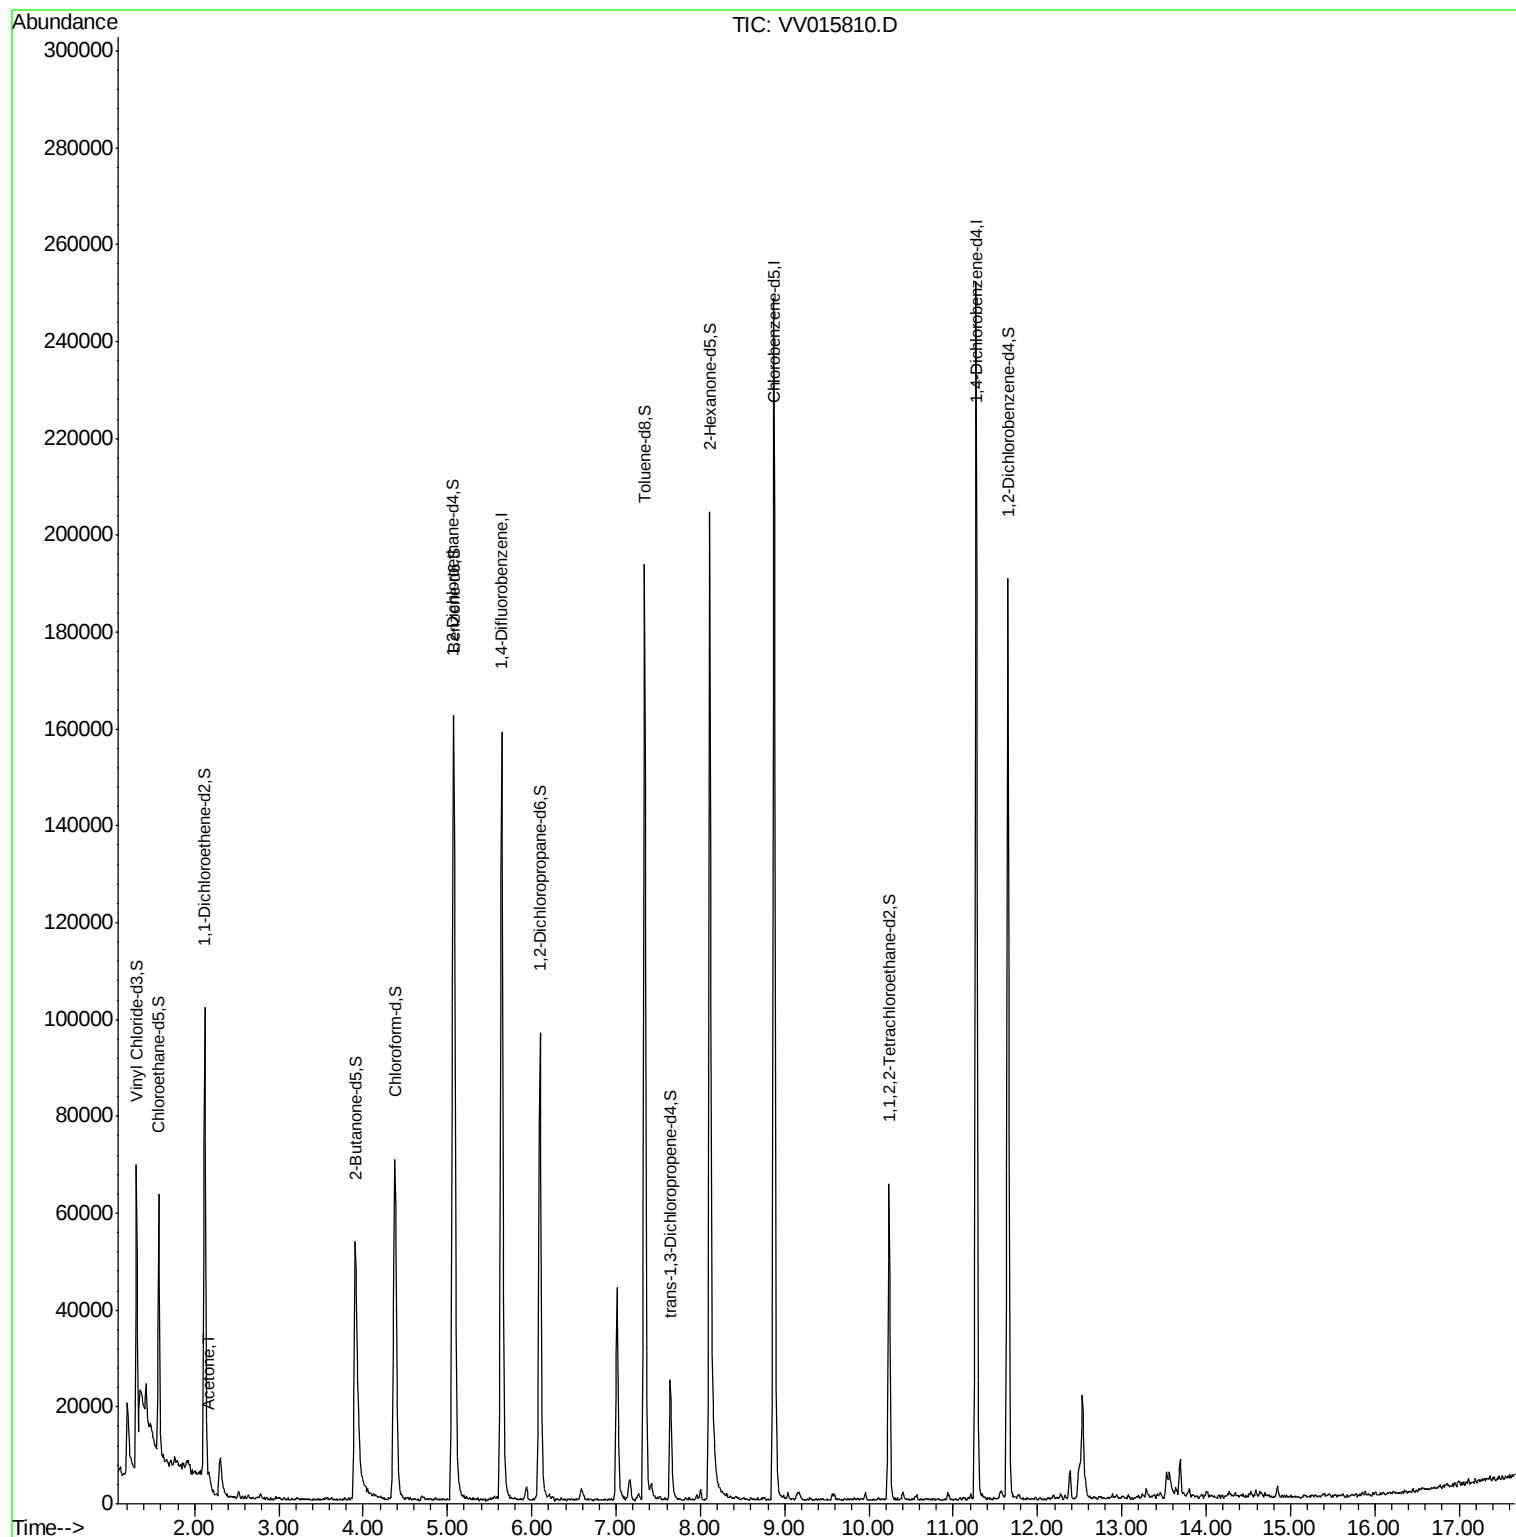

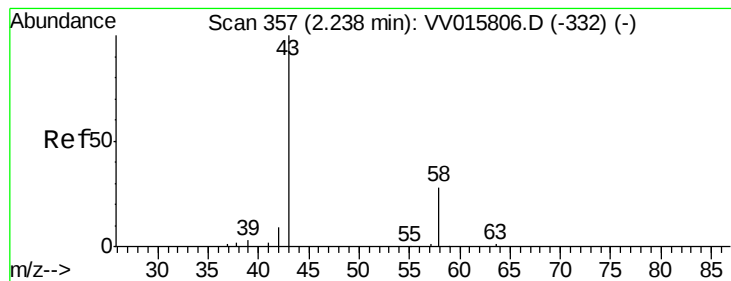

#13
 Acetone
 Concen: 1.813 ug/L
 RT: 2.18 min Scan# 339
 Delta R.T. -0.04 min
 Lab File: VV015810.D
 Acq: 30 Apr 2020 00:06

Instrument :
 MSVOA_V
 ClientSampleId :
 ETKR3

Tot Ion: 43 Resp: 2696
 Ion Ratio Lower Upper
 43 100
 58 26.3 0.0 57.6

