

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV042920\
 Data File : VV015785.D
 Acq On : 29 Apr 2020 12:20
 Operator : SY/MD
 Sample : L2419-04DL 400X
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AF1DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.1

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	61	69	79	rBV	66033	68644	16.63%	1.728%
2	1.573	142	150	163	rBV	55907	68565	16.61%	1.726%
3	2.116	310	319	330	rVB	102509	143840	34.84%	3.621%
4	2.521	435	445	454	rBV	5992	10057	2.44%	0.253%
5	3.955	875	891	924	rBV3	33539	168352	40.78%	4.238%
6	4.376	1001	1022	1052	rVB2	64132	181810	44.04%	4.577%
7	5.071	1221	1238	1263	rBV2	168179	412804	100.00%	10.392%
8	5.640	1401	1415	1434	rBV2	158873	320655	77.68%	8.072%
9	5.933	1496	1506	1518	rVB9	4011	8073	1.96%	0.203%
10	6.093	1543	1556	1579	rBV	97617	203075	49.19%	5.112%
11	7.010	1828	1841	1864	rBV	44650	84354	20.43%	2.124%
12	7.338	1931	1943	1965	rBV	193206	340366	82.45%	8.568%
13	7.646	2025	2039	2051	rBV	27299	47337	11.47%	1.192%
14	7.997	2128	2148	2168	rBV	181911	308910	74.83%	7.777%
15	8.116	2172	2185	2211	rBV2	194364	397862	96.38%	10.016%
16	8.875	2407	2421	2445	rBV	249304	407213	98.65%	10.251%
17	10.238	2833	2845	2861	rBV	62225	99358	24.07%	2.501%
18	11.270	3155	3166	3184	rBV	248346	390731	94.65%	9.836%
19	11.646	3271	3283	3297	rBV	193268	305870	74.10%	7.700%
20	12.270	3465	3477	3487	rBV4	2316	4449	1.08%	0.112%


Sum of corrected areas: 3972325

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV042920\
Data File : VV015785.D
Acq On : 29 Apr 2020 12:20
Operator : SY/MD
Sample : L2419-04DL 400X
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF1DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

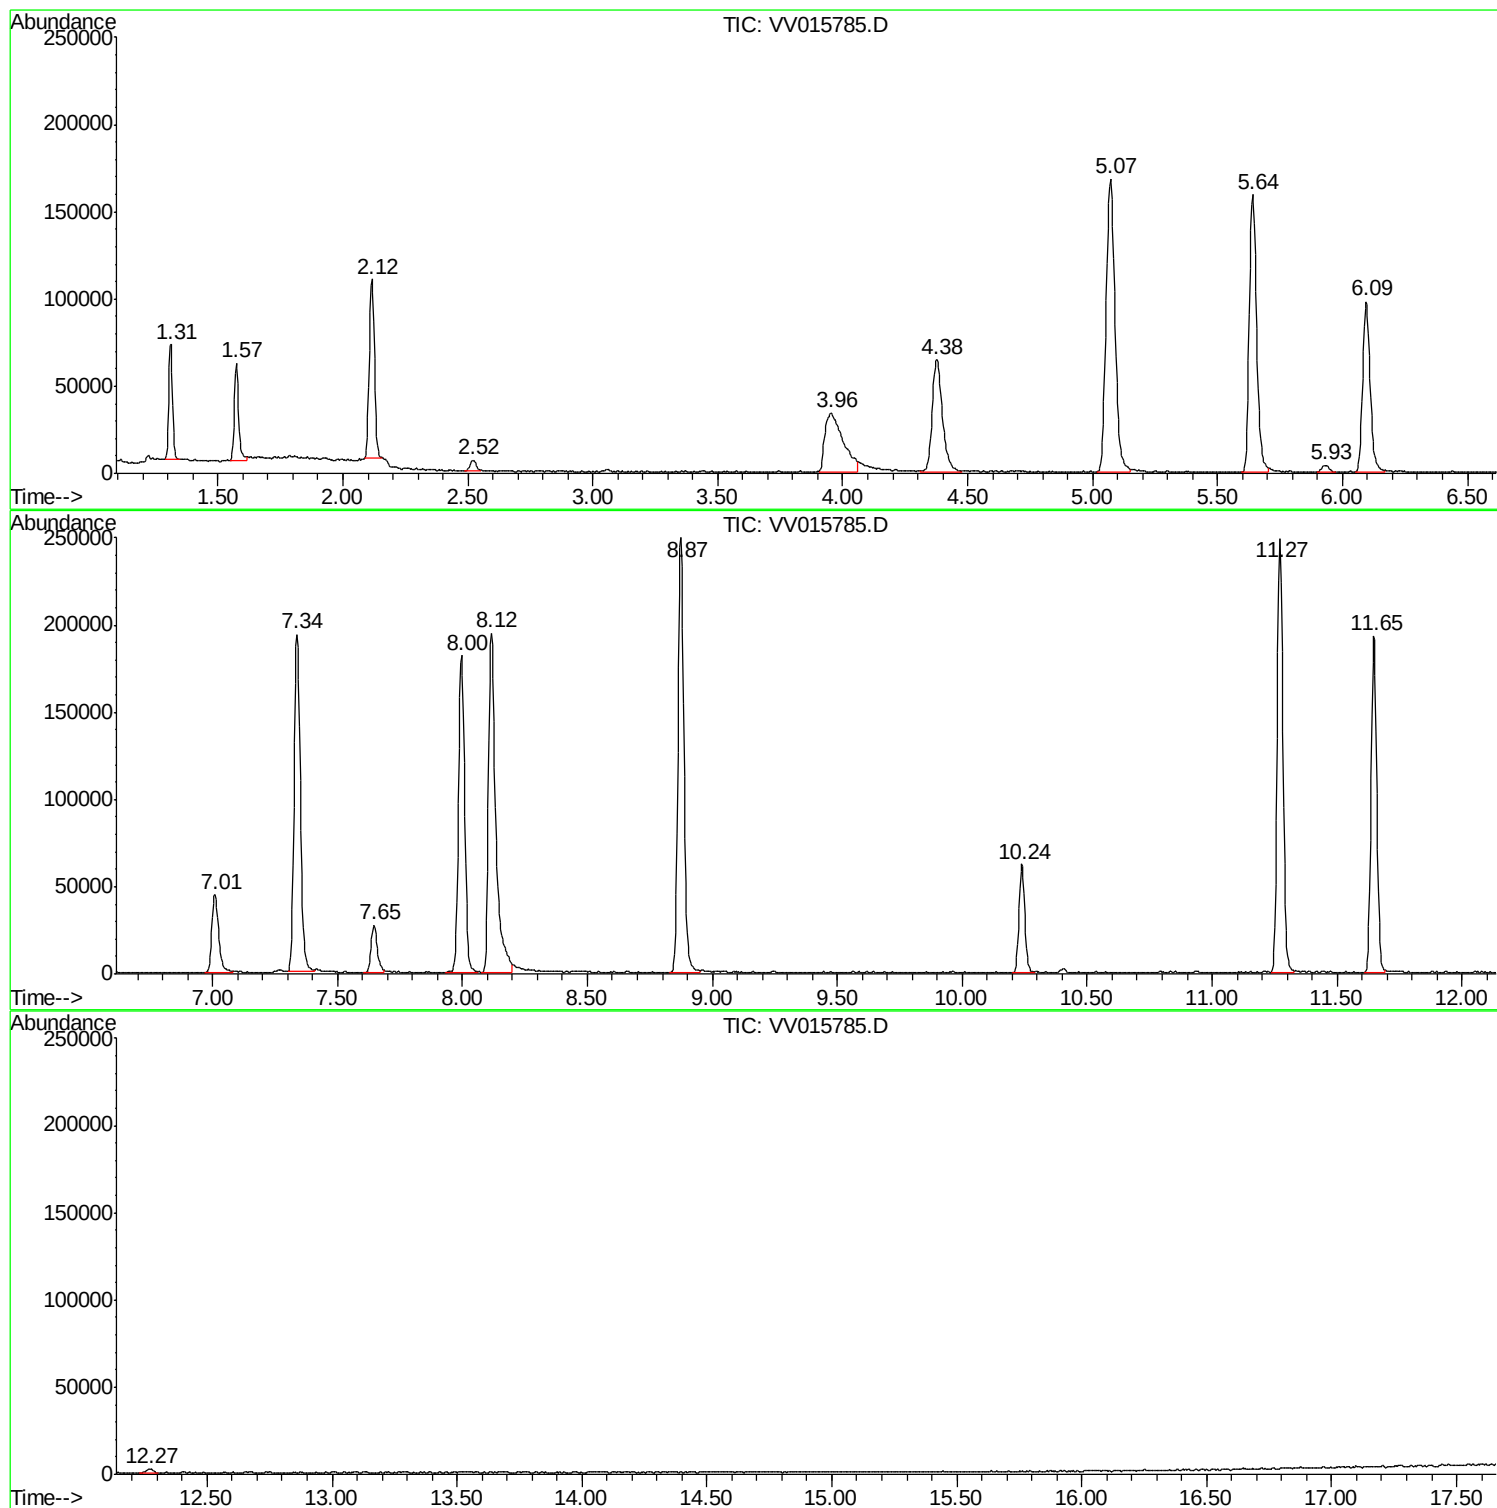

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV042920\
Data File : VV015785.D
Acq On : 29 Apr 2020 12:20
Operator : SY/MD
Sample : L2419-04DL 400X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF1DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV042920\
Data File : VV015785.D
Acq On : 29 Apr 2020 12:20
Operator : SY/MD
Sample : L2419-04DL 400X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF1DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc