

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV042920\
 Data File : VV015802.D
 Acq On : 29 Apr 2020 19:00
 Operator : SY/MD
 Sample : L2421-06DL 10X
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFS7DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.1

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	62	70	87	rVB	67987	72838	13.00%	1.557%
2	1.576	144	151	167	rVB	57145	68003	12.14%	1.453%
3	2.123	311	321	337	rVB	103841	156296	27.91%	3.341%
4	2.524	438	446	458	rVB3	4351	7480	1.34%	0.160%
5	2.785	517	527	539	rBV6	7569	14446	2.58%	0.309%
6	3.936	865	885	915	rBV3	140402	470838	84.06%	10.064%
7	4.376	1006	1022	1052	rBV	69271	185670	33.15%	3.969%
8	5.074	1222	1239	1267	rBV2	168421	428197	76.45%	9.152%
9	5.643	1401	1416	1445	rBV	162325	333582	59.56%	7.130%
10	5.939	1495	1508	1543	rVB	284510	560100	100.00%	11.972%
11	6.093	1543	1556	1574	rBV	98053	205664	36.72%	4.396%
12	7.010	1830	1841	1865	rBV2	46058	88626	15.82%	1.894%
13	7.338	1932	1943	1961	rBV	200513	350098	62.51%	7.483%
14	7.412	1961	1966	1977	rVB5	4237	7473	1.33%	0.160%
15	7.643	2028	2038	2066	rBV2	26602	52010	9.29%	1.112%
16	8.000	2141	2149	2162	rVB8	4936	8290	1.48%	0.177%
17	8.113	2173	2184	2217	rBV2	197799	408459	72.93%	8.730%
18	8.875	2409	2421	2444	rBV	256809	426603	76.17%	9.118%
19	9.566	2629	2636	2656	rBV7	3616	9103	1.63%	0.195%
20	10.238	2834	2845	2857	rBV	65349	102806	18.35%	2.197%
21	11.270	3156	3166	3186	rBV	260326	406818	72.63%	8.695%
22	11.646	3271	3283	3304	rBV	197461	315171	56.27%	6.736%


Sum of corrected areas: 4678571

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV042920\
Data File : VV015802.D
Acq On : 29 Apr 2020 19:00
Operator : SY/MD
Sample : L2421-06DL 10X
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFSA7DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

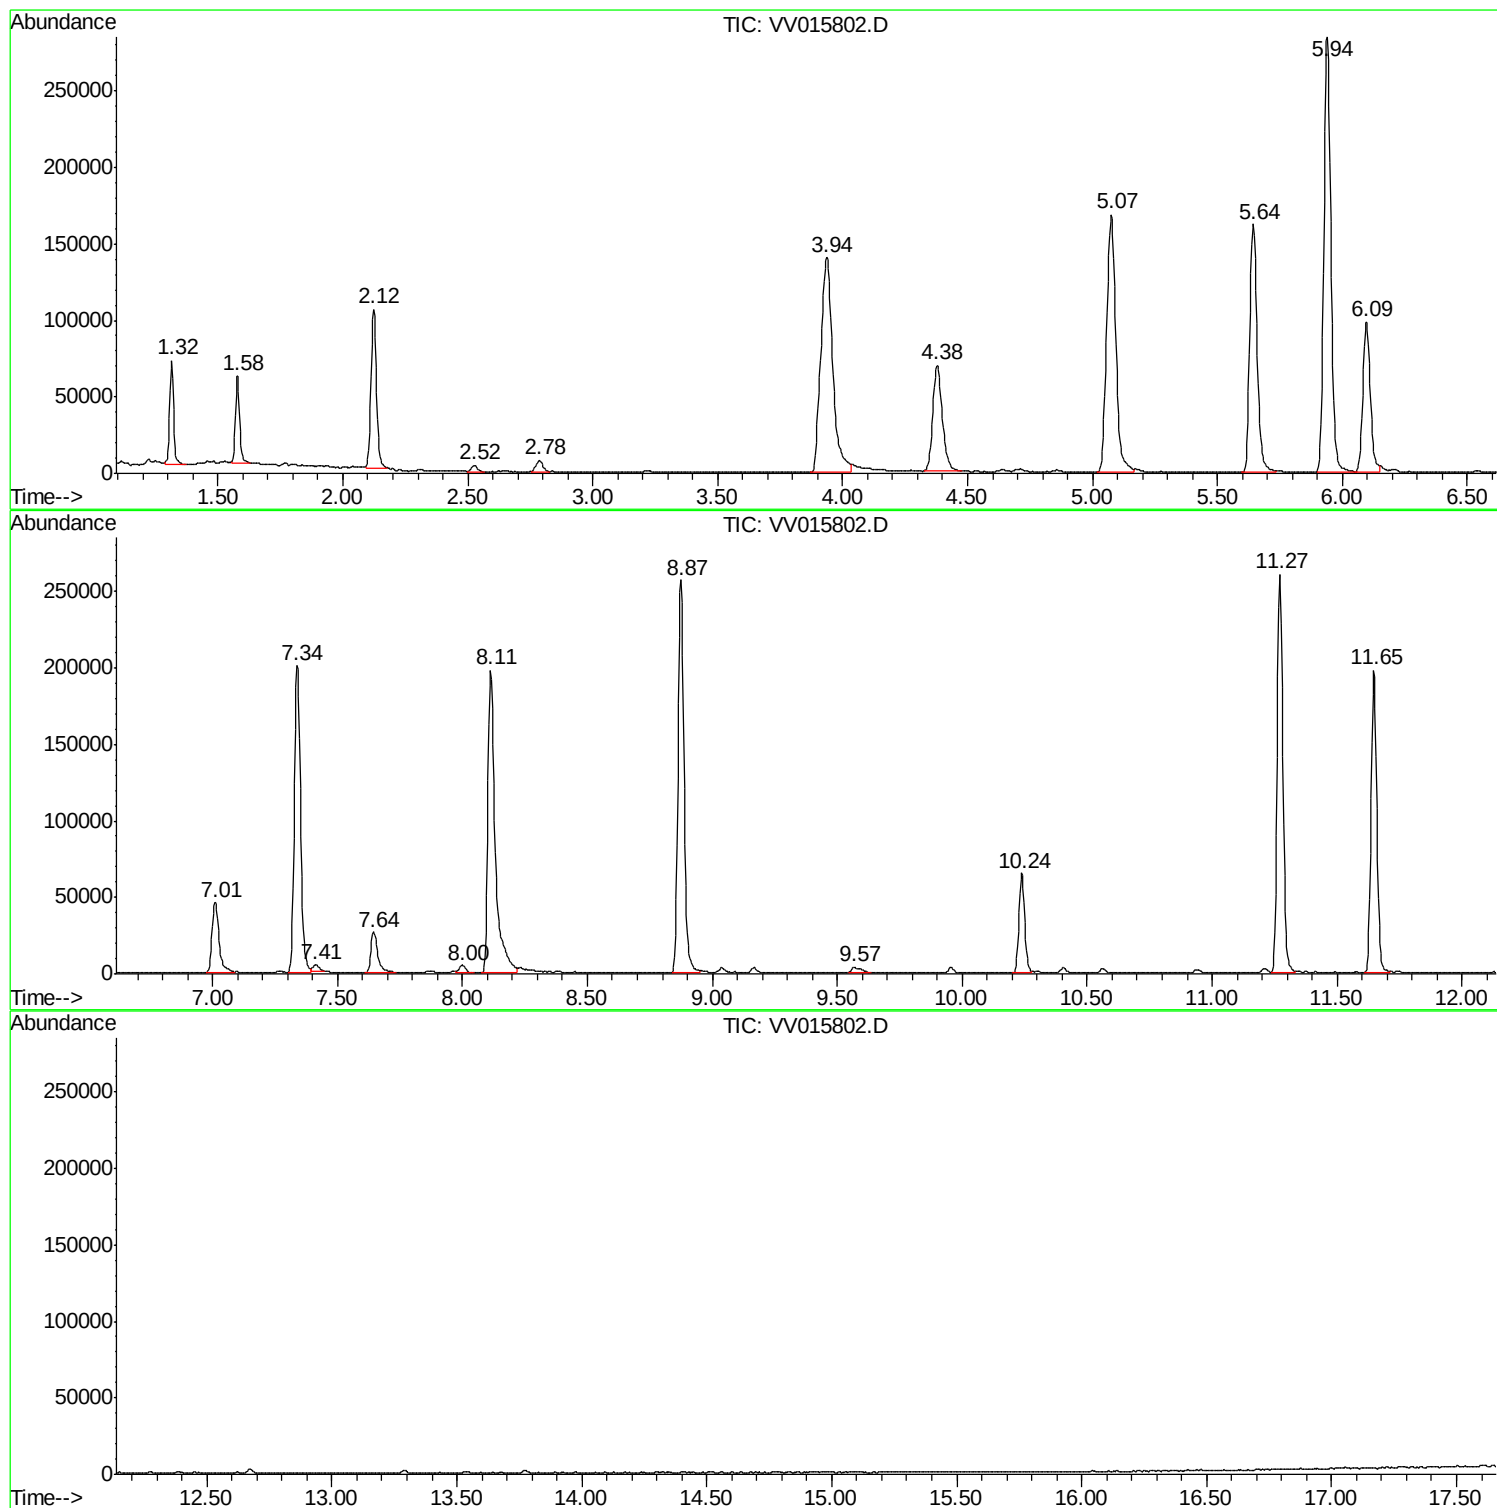

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV042920\
Data File : VV015802.D
Acq On : 29 Apr 2020 19:00
Operator : SY/MD
Sample : L2421-06DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFS7DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV042920\
Data File : VV015802.D
Acq On : 29 Apr 2020 19:00
Operator : SY/MD
Sample : L2421-06DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFS7DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc