

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV042920\
 Data File : VV015823.D
 Acq On : 30 Apr 2020 05:14
 Operator : SY/MD
 Sample : L2431-18
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETKS7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.1

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC: VV015826.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.222	34	41	47	rBV	260298	229110	55.83%	5.782%
2	1.312	60	69	79	rVB2	64461	81935	19.97%	2.068%
3	1.392	88	94	101	rBV3	4872	7210	1.76%	0.182%
4	1.576	144	151	162	rVB	55457	62717	15.28%	1.583%
5	2.122	310	321	333	rBV	98417	152223	37.09%	3.842%
6	2.183	334	340	355	rVB	12359	22759	5.55%	0.574%
7	2.515	433	443	444	rBV4	6869	7858	1.91%	0.198%
8	2.547	450	453	464	rVB2	11970	15784	3.85%	0.398%
9	2.778	514	525	541	rVB5	8468	18717	4.56%	0.472%
10	2.971	576	585	601	rVB6	1902	4266	1.04%	0.108%
11	3.910	865	877	904	rBV2	51430	148222	36.12%	3.741%
12	4.380	1006	1023	1050	rBV	68208	180407	43.96%	4.553%
13	5.074	1219	1239	1263	rBV2	164385	410362	100.00%	10.357%
14	5.643	1402	1416	1441	rBV	156112	314410	76.62%	7.935%
15	5.929	1496	1505	1516	rVB6	2739	5684	1.39%	0.143%
16	6.096	1543	1557	1585	rVB	96388	200128	48.77%	5.051%
17	7.010	1829	1841	1856	rBV	41222	76556	18.66%	1.932%
18	7.338	1932	1943	1964	rBV	196360	350369	85.38%	8.843%
19	7.646	2030	2039	2056	rBV	23736	42521	10.36%	1.073%
20	8.112	2173	2184	2222	rBV	206101	407537	99.31%	10.285%
21	8.273	2227	2234	2246	rVB9	4992	9133	2.23%	0.230%
22	8.874	2409	2421	2442	rBV	236751	390422	95.14%	9.853%
23	9.161	2503	2510	2519	rBV5	2769	4190	1.02%	0.106%
24	9.836	2707	2720	2729	rBV8	4713	8452	2.06%	0.213%
25	10.238	2834	2845	2859	rBV	61203	97635	23.79%	2.464%
26	11.273	3154	3167	3187	rBV	245470	386247	94.12%	9.748%
27	11.646	3272	3283	3300	rBV	192321	307042	74.82%	7.749%
28	12.370	3499	3508	3520	rBV5	12698	20420	4.98%	0.515%


Sum of corrected areas: 3962316

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV042920\
Data File : VV015823.D
Acq On : 30 Apr 2020 05:14
Operator : SY/MD
Sample : L2431-18
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETKS7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

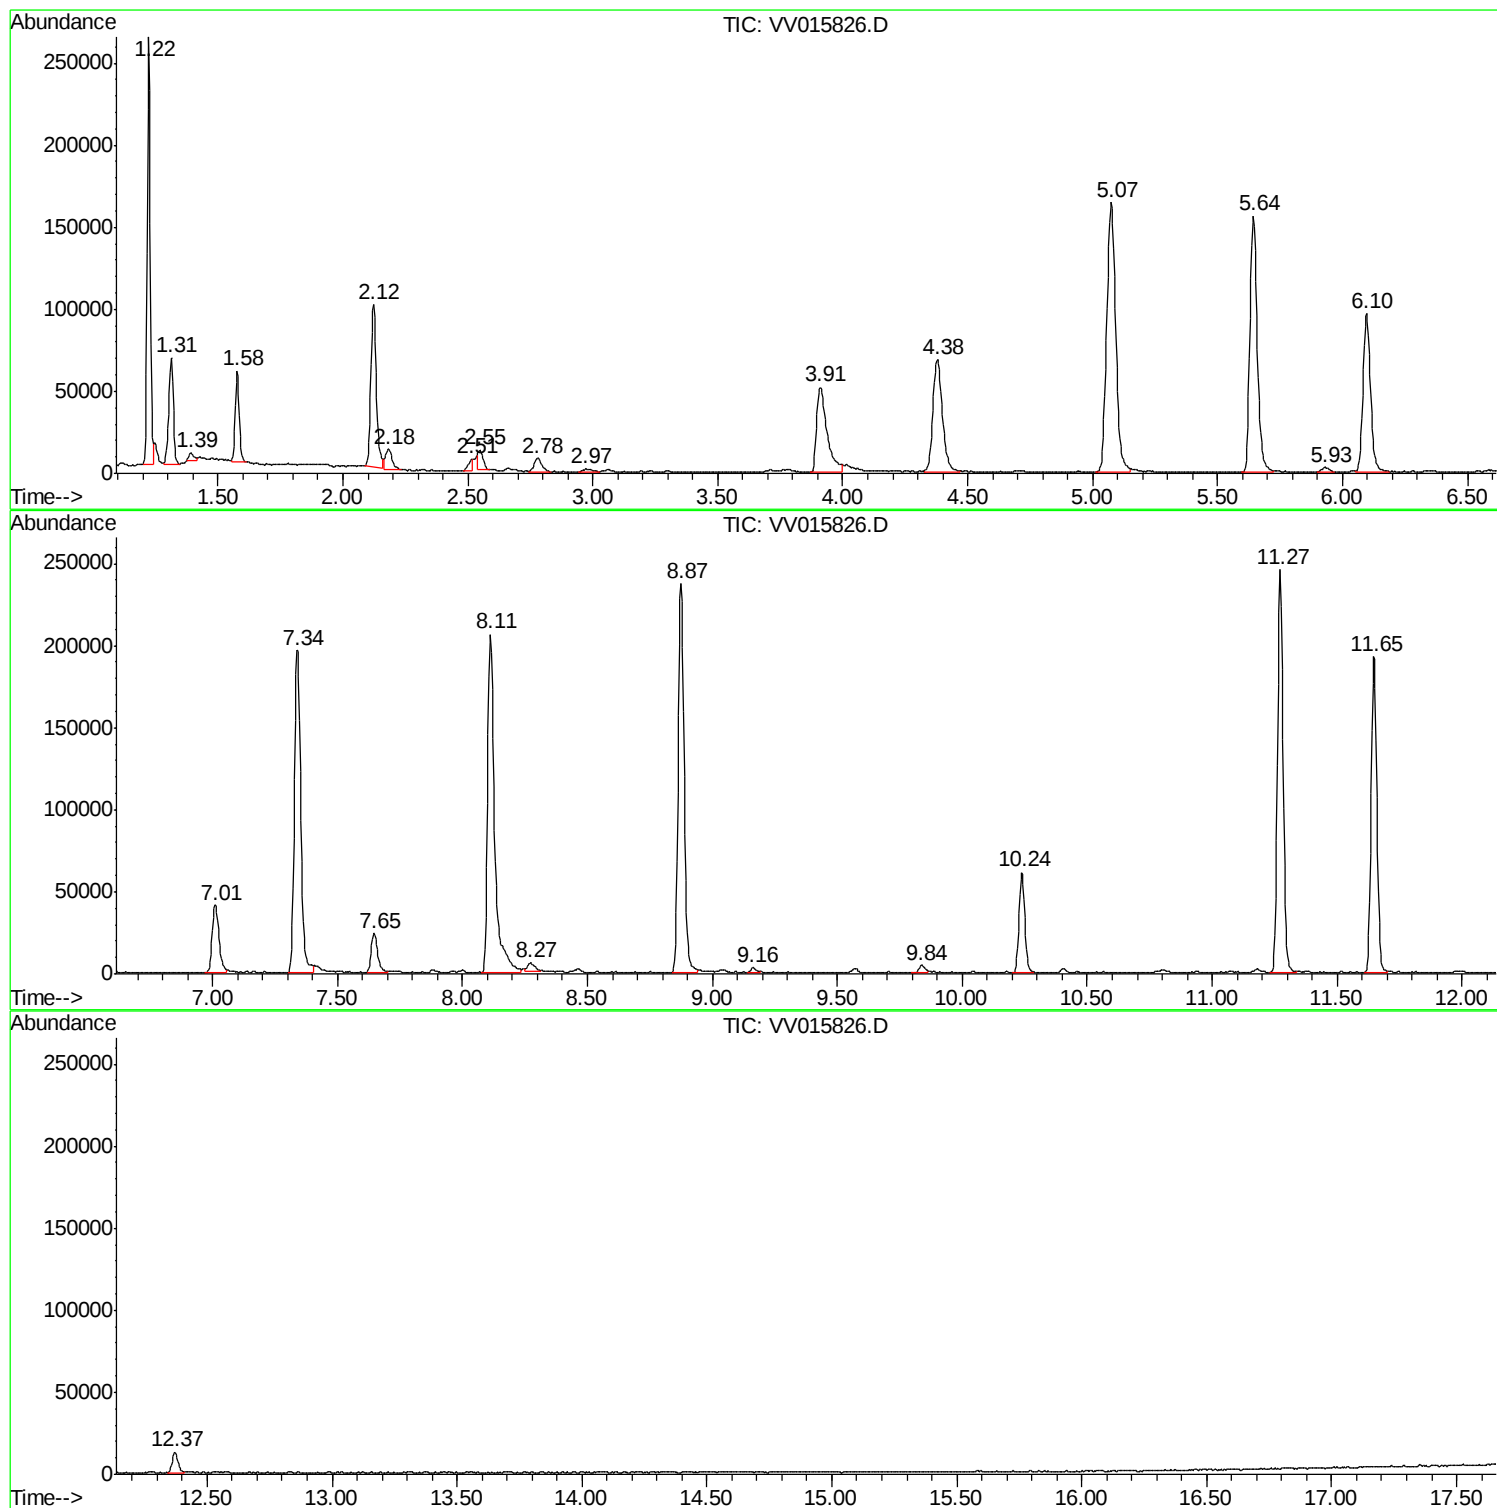

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV042920\
Data File : VV015823.D
Acq On : 30 Apr 2020 05:14
Operator : SY/MD
Sample : L2431-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETKS7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV042920\
Data File : VV015823.D
Acq On : 30 Apr 2020 05:14
Operator : SY/MD
Sample : L2431-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETKS7

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
