


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV042920\
 Data File : VV015781.D
 Acq On : 29 Apr 2020 10:02
 Operator : SY/MD
 Sample : BFB46
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB46

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Apr 30 01:35:08 2020

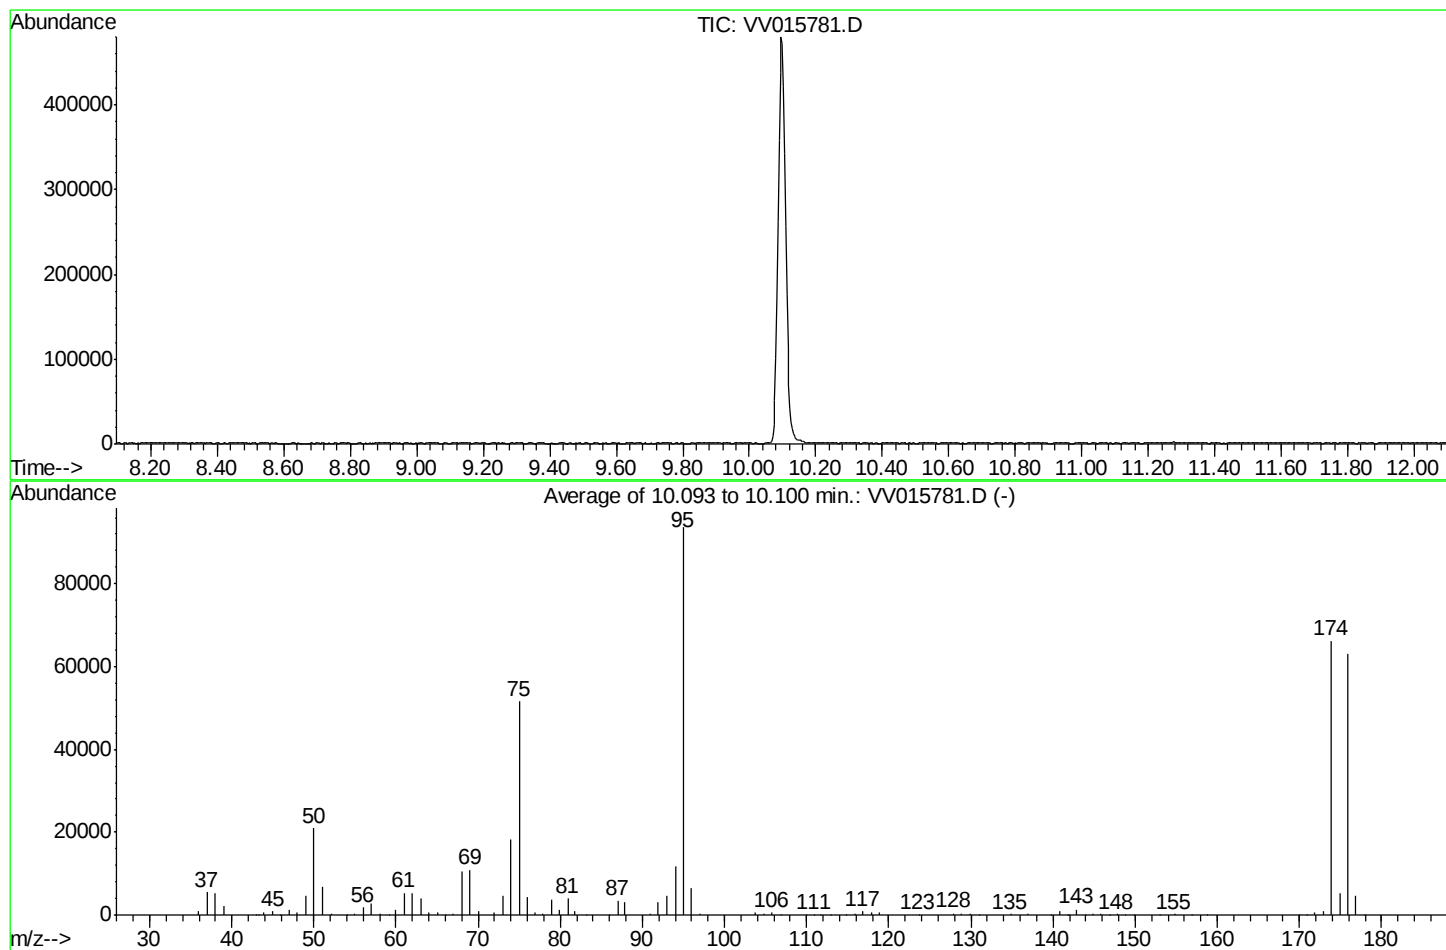

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2788

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.3	20890	PASS
75	95	30	80	55.1	51594	PASS
95	95	100	100	100.0	93640	PASS
96	95	5	9	6.9	6441	PASS
173	174	0.00	2	1.5	966	PASS
174	95	50	120	70.8	66309	PASS
175	174	5	9	7.9	5244	PASS
176	174	95	101	95.0	63024	PASS
177	176	5	9	7.5	4729	PASS

m/z	Abundance
36.00	928.0
37.00	5370.0
38.00	5089.0
39.00	1950.0
39.90	430.0
43.00	131.0
43.90	1113.0
45.00	845.0
45.80	160.0
47.00	1025.0
47.90	768.0
49.00	4398.0
50.00	20048.0
51.00	6567.0
52.10	254.0
54.00	103.0
55.00	247.0
56.00	1678.0
57.00	2694.0
58.00	170.0
59.20	130.0
60.00	1150.0
61.00	5083.0
62.00	5183.0
63.00	3912.0
63.90	556.0
65.00	471.0
66.00	110.0
67.00	323.0
68.00	10176.0
69.00	10421.0
70.00	955.0
71.90	595.0
73.00	4094.0
74.00	17096.0
75.00	48920.0
76.00	4554.0
77.00	648.0
77.90	314.0
78.90	3601.0
79.90	1152.0
80.90	3682.0
81.80	800.0
85.90	138.0
87.00	3258.0
87.90	3131.0
90.90	453.0
91.90	2786.0
93.00	4233.0
94.00	10996.0
95.00	88648.0
96.00	6018.0
97.00	148.0
103.80	540.0
104.80	156.0
105.80	511.0
106.80	129.0
110.90	130.0
111.70	156.0
114.90	146.0
115.90	418.0
116.80	731.0
117.90	467.0
118.90	614.0
123.60	119.0
127.90	396.0
128.80	184.0
129.90	306.0
131.00	143.0
134.80	237.0
136.80	187.0
139.80	118.0
140.90	974.0
141.70	145.0
142.90	1250.0
144.90	227.0
145.70	223.0
146.90	121.0
147.80	179.0
149.90	120.0
152.90	135.0
154.80	286.0
158.80	102.0
169.90	123.0
170.90	112.0
171.90	502.0
173.00	956.0
173.90	60960.0
175.00	4883.0
175.90	58488.0
176.90	4484.0
177.90	118.0

Instrument :
MSVOA_V
ClientSampleId :
BFB46

m/z	Abundance
35.90	1030.0
37.00	5489.0
38.00	4959.0
39.00	2103.0
39.90	427.0
42.90	151.0
43.90	1120.0
45.00	958.0
45.90	123.0
47.10	1186.0
48.00	639.0
49.00	4702.0
50.00	21064.0
51.00	6510.0
52.10	216.0
54.00	121.0
55.00	313.0
56.00	1809.0
57.00	2690.0
58.00	219.0
60.00	1081.0
61.00	5325.0
62.00	4904.0
63.00	4252.0
63.90	426.0
65.10	545.0
67.00	281.0
68.00	10657.0
69.00	11088.0
70.00	852.0
72.00	631.0
73.00	4834.0
74.00	18648.0
75.00	52472.0
76.00	4241.0
76.90	786.0
77.90	411.0
78.90	3950.0
79.90	1086.0
80.90	4026.0
81.80	870.0
83.10	106.0
85.90	147.0
87.00	3541.0
87.90	3090.0
90.90	476.0
92.00	3038.0
93.00	4760.0
94.00	12295.0
95.00	95352.0
96.00	6673.0
97.10	187.0
103.80	540.0
104.80	247.0
105.80	590.0
106.80	117.0
109.90	140.0
110.90	168.0
111.70	126.0
112.80	146.0
114.80	109.0
115.90	420.0
116.90	908.0
118.00	472.0
118.90	584.0
127.90	400.0
128.90	205.0
129.80	402.0
130.90	141.0
134.80	261.0
136.90	236.0
140.80	1045.0
141.80	115.0
142.90	1289.0
144.00	104.0
144.90	217.0
145.80	239.0
147.80	247.0
148.80	102.0
149.90	103.0
153.00	134.0
154.90	253.0
156.90	185.0
171.00	105.0
171.90	526.0
173.00	948.0
173.90	69176.0
174.90	5419.0
175.90	65304.0
176.90	4740.0
177.90	112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB46

m/z	Abundance
35.90	1035.0
37.00	5636.0
38.00	5332.0
39.00	2122.0
39.90	417.0
43.20	150.0
43.90	1169.0
45.00	923.0
45.80	138.0
47.00	1146.0
48.00	743.0
49.00	4856.0
50.00	21560.0
51.00	6944.0
52.10	224.0
54.00	120.0
55.00	301.0
56.00	1829.0
57.00	2846.0
58.00	222.0
59.10	114.0
60.00	1166.0
61.00	5503.0
62.00	5427.0
63.00	4339.0
63.90	529.0
65.00	533.0
66.00	114.0
67.00	311.0
68.00	10841.0
69.00	11350.0
70.00	991.0
72.00	682.0
73.00	4692.0
74.00	18800.0
75.00	53392.0
76.00	4583.0
77.00	774.0
77.90	389.0
78.90	4005.0
79.90	1223.0
80.90	4069.0
81.80	846.0
85.90	146.0
87.00	3617.0
87.90	3177.0
90.90	498.0
92.00	3077.0
93.00	4724.0
94.00	12196.0
95.00	96920.0
96.00	6634.0
97.10	176.0
103.80	560.0
104.80	225.0
105.80	596.0
106.80	135.0
109.90	139.0
110.90	157.0
111.70	154.0
112.90	122.0
114.90	132.0
115.90	459.0
116.90	862.0
117.90	494.0
118.90	635.0
127.90	425.0
128.80	193.0
129.80	363.0
131.00	159.0
134.90	284.0
136.80	222.0
140.80	1015.0
141.90	126.0
142.90	1353.0
145.00	247.0
145.80	247.0
146.80	126.0
147.80	215.0
149.90	130.0
153.00	149.0
154.80	290.0
156.90	153.0
169.90	108.0
170.90	110.0
171.90	529.0
173.00	994.0
173.90	68792.0
174.90	5430.0
175.90	65280.0
176.90	4964.0
177.90	120.0

Instrument :
MSVOA_V
ClientSampleId :
BFB46

Scan 2788 (10.055 min): VV015781.D
BFB46

m/z	Abundance
39.90	431.0
43.90	515.0

Instrument :
MSVOA_V
ClientSampleId :
BFB46