

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042921\
 Data File : VV021220.D
 Acq On : 29 Apr 2021 15:08
 Operator : SY/MD
 Sample : VV0429WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Apr 30 05:56:41 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 30 05:55:34 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	560756	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	541783	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.256	152	269304	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	156632	33.99	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 67.98%			
7) Chloroethane-d5	1.571	69	130177	38.40	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 76.80%			
11) 1,1-Dichloroethene-d2	2.108	63	260582	30.66	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 61.32%			
21) 2-Butanone-d5	3.899	46	210472	93.54	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 93.54%			
24) Chloroform-d	4.352	84	376944	45.89	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 91.78%			
26) 1,2-Dichloroethane-d4	5.037	65	290622	55.66	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 111.32%			
32) Benzene-d6	5.053	84	669423	46.39	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 92.78%			
36) 1,2-Dichloropropane-d6	6.076	67	188307	43.72	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 87.44%			
41) Toluene-d8	7.320	98	656542	47.01	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 94.02%			
43) trans-1,3-Dichloroprop...	7.532	79	645	0.27	ug/L	-0.09
Spiked Amount 50.000	Range 60 - 125		Recovery = 0.54%#			
47) 2-Hexanone-d5	8.092	63	151933	88.94	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 88.94%			
56) 1,1,2,2-Tetrachloroeth...	10.220	84	266917	41.09	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 82.18%			
66) 1,2-Dichlorobenzene-d4	11.632	152	294154	55.29	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 110.58%			
Target Compounds					Qvalue	
68) 1,2-Dibromo-3-chloropr...	12.059	75	2207	1.62	ug/L	# 34


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042921\
Data File : VV021220.D
Acq On : 29 Apr 2021 15:08
Operator : SY/MD
Sample : VV0429WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Apr 30 05:56:41 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 30 05:55:34 2021
Response via : Initial Calibration

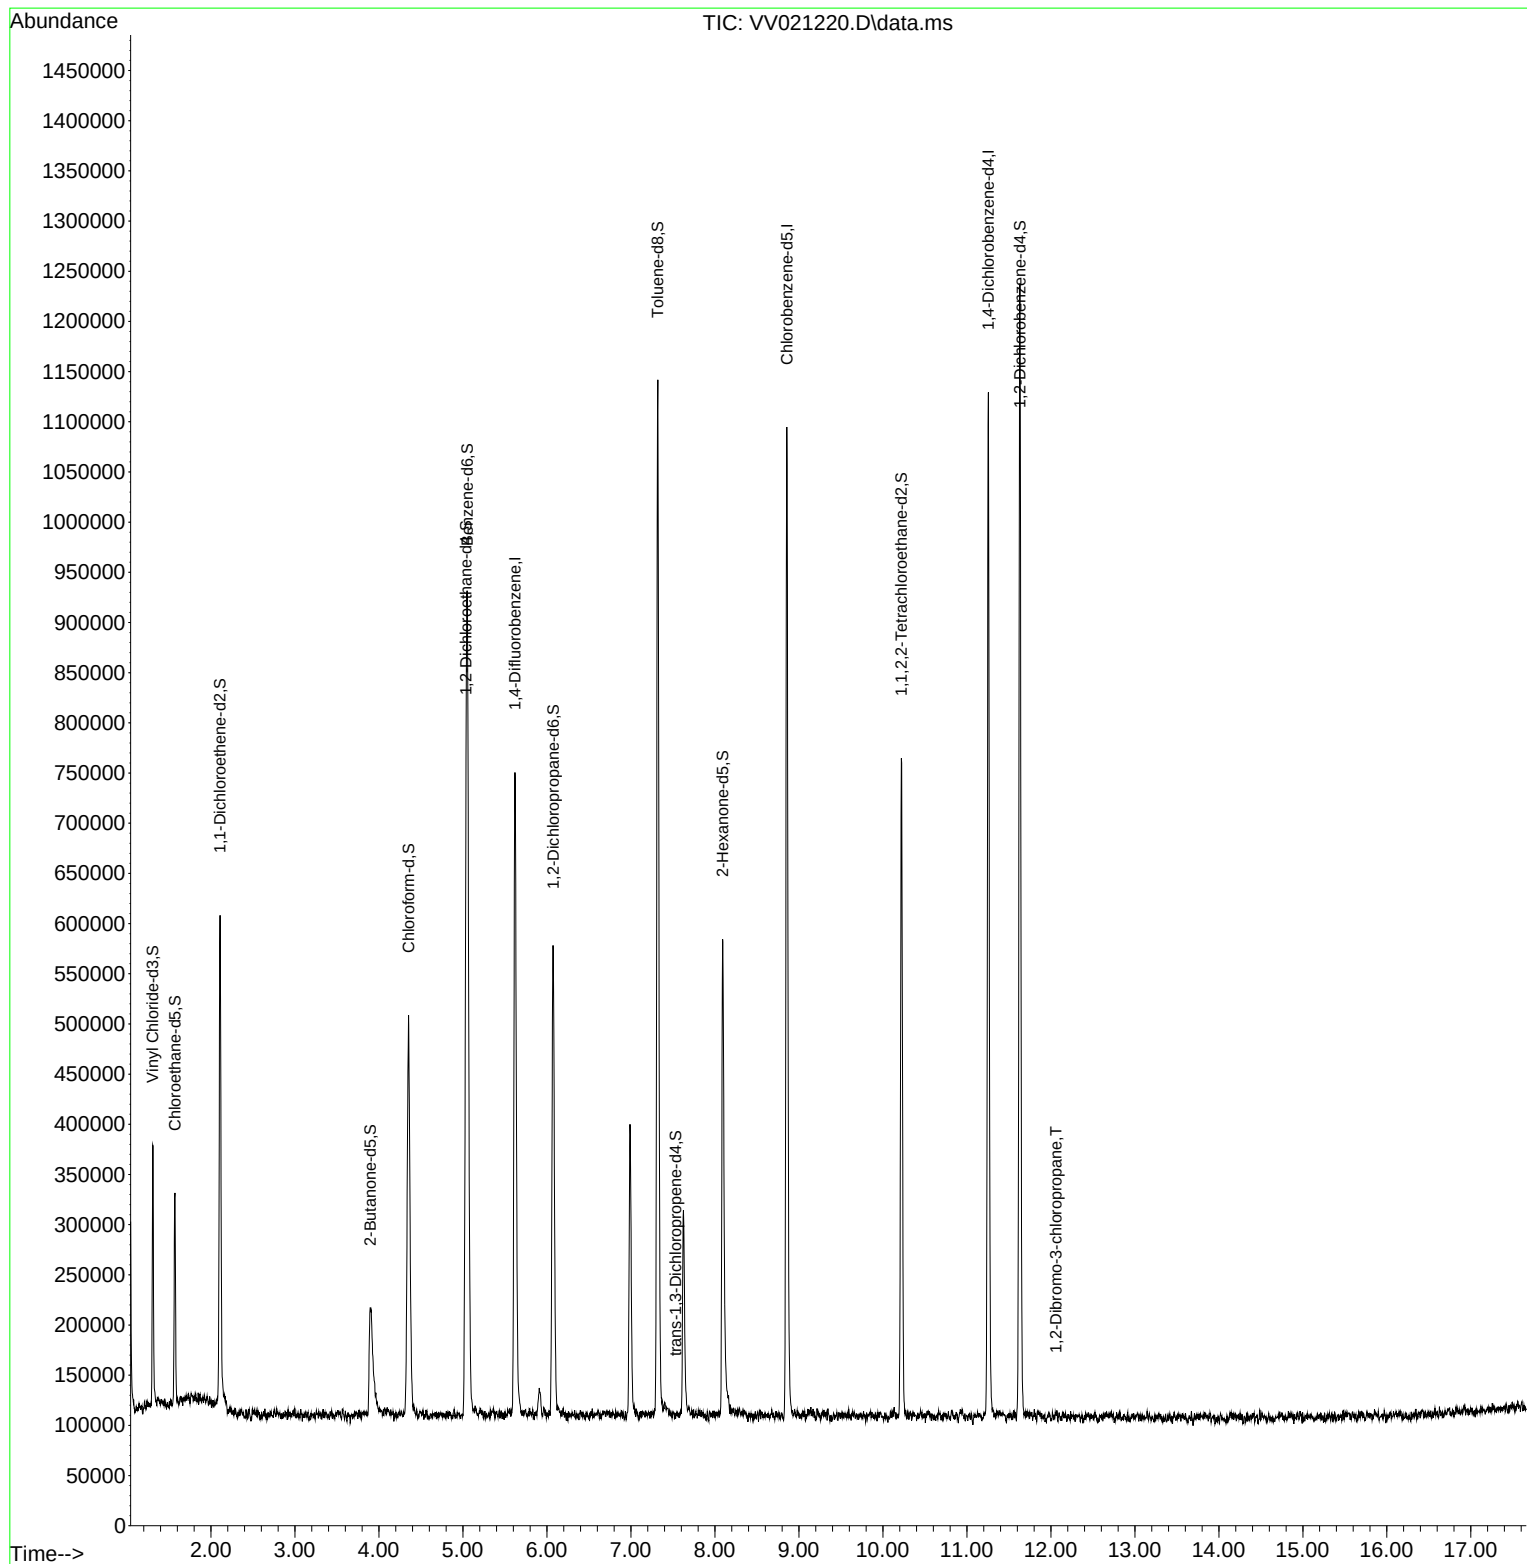

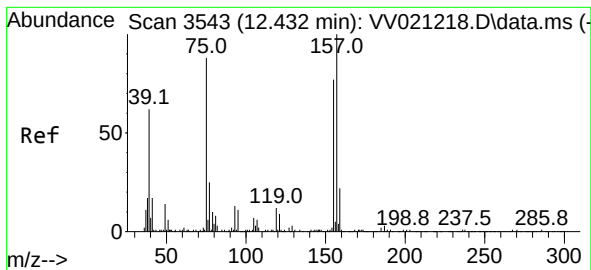

#68
 1,2-Dibromo-3-chloropropane
 Concen: 1.62 ug/L
 RT: 12.059 min Scan# 3427
 Delta R.T. -0.373 min
 Lab File: VV021220.D
 Acq: 29 Apr 2021 15:08

Instrument :
 MSVOA_V
 ClientSampleId :

Tgt Ion: 75 Resp: 2207
 Ion Ratio Lower Upper
 75 100
 155 34.7 72.8 109.2#
 157 39.1 94.6 142.0#

