

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042921\
 Data File : VV021221.D
 Acq On : 29 Apr 2021 15:31
 Operator : SY/MD
 Sample : M2123-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Apr 30 05:56:53 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 30 05:55:34 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	545691	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	535098	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.255	152	256911	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	157969	35.23	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 70.46%			
7) Chloroethane-d5	1.571	69	125803	38.14	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 76.28%			
11) 1,1-Dichloroethene-d2	2.108	63	255852	30.94	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 61.88%			
21) 2-Butanone-d5	3.902	46	206829	94.46	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 94.46%			
24) Chloroform-d	4.352	84	375327	46.95	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 93.90%			
26) 1,2-Dichloroethane-d4	5.037	65	289989	57.07	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 114.14%			
32) Benzene-d6	5.053	84	673491	47.26	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 94.52%			
36) 1,2-Dichloropropane-d6	6.072	67	187974	44.19	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 88.38%			
41) Toluene-d8	7.320	98	650316	47.15	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 94.30%			
43) trans-1,3-Dichloroprop...	7.876	79	337	0.14	ug/L	0.25
Spiked Amount 50.000	Range 60 - 125		Recovery = 0.28%#			
47) 2-Hexanone-d5	8.095	63	152163	90.19	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 90.19%			
56) 1,1,2,2-Tetrachloroeth...	10.220	84	266113	41.48	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 82.96%			
66) 1,2-Dichlorobenzene-d4	11.632	152	284549	56.07	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 112.14%			
Target Compounds					Qvalue	
68) 1,2-Dibromo-3-chloropr...	12.435	75	1286	0.99	ug/L #	27


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042921\
Data File : VV021221.D
Acq On : 29 Apr 2021 15:31
Operator : SY/MD
Sample : M2123-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Apr 30 05:56:53 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 30 05:55:34 2021
Response via : Initial Calibration

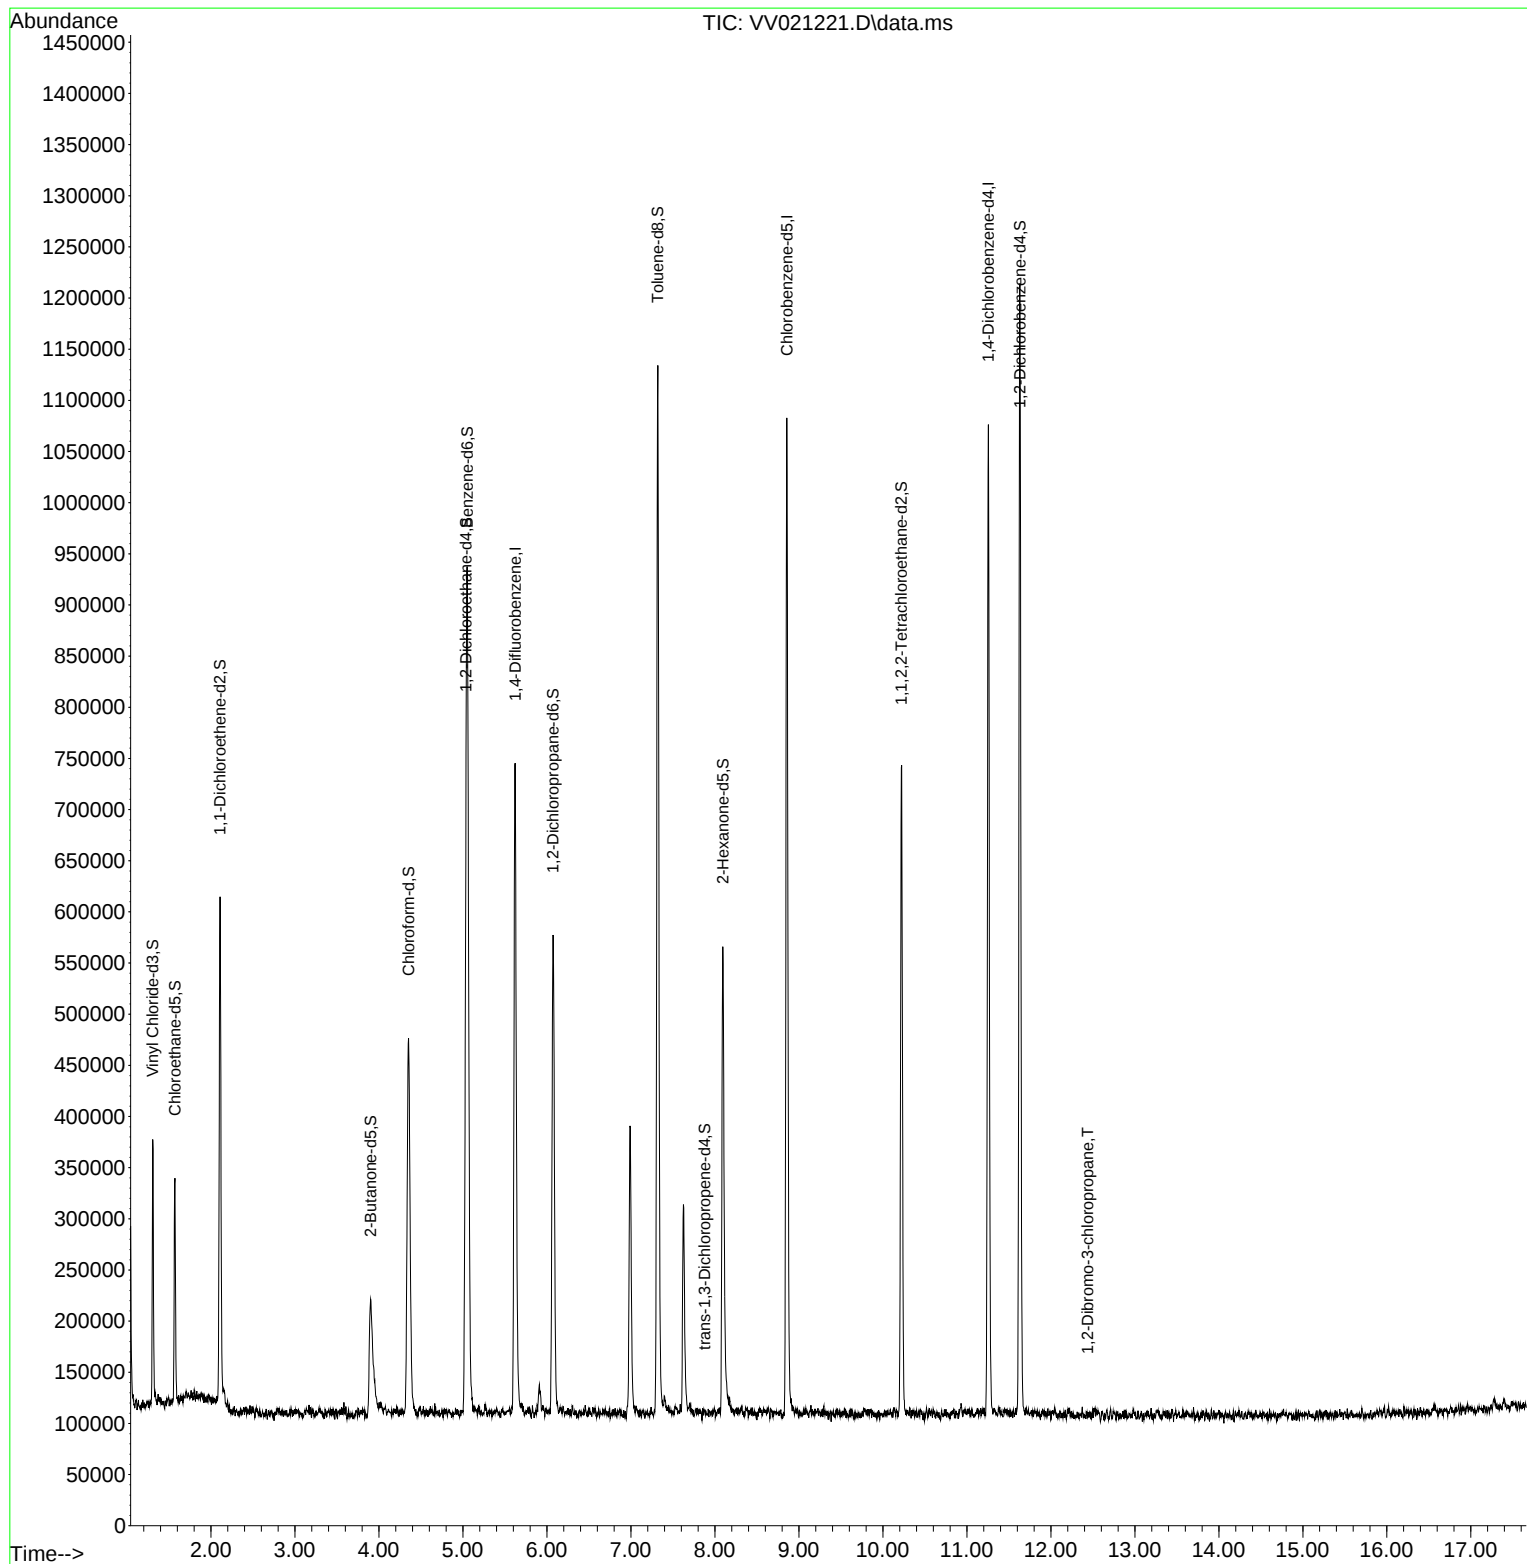

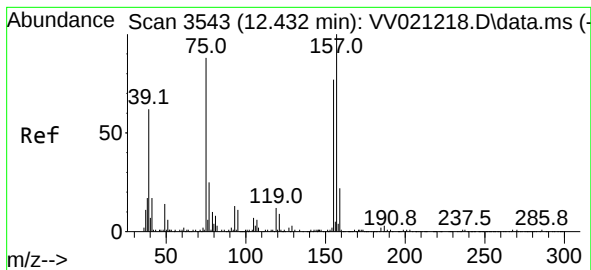

#68

1,2-Dibromo-3-chloropropane

Concen: 0.99 ug/L

RT: 12.435 min Scan# 3544

Delta R.T. 0.003 min

Lab File: VV021221.D

Acq: 29 Apr 2021 15:31

Tgt Ion: 75 Resp: 1286

Ion Ratio Lower Upper

75 100

155 31.0 72.8 109.2#

157 28.7 94.6 142.0#

Instrument :

MSVOA_V

ClientSampleId :

