

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042921\
 Data File : VV021223.D
 Acq On : 29 Apr 2021 16:17
 Operator : SY/MD
 Sample : M2177-05ME
 Misc : 5.49g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Apr 30 05:57:20 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 30 05:55:34 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	591303	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.860	117	566430	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.259	152	331073	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	139321	28.67	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	57.34%#
7) Chloroethane-d5	1.568	69	74911	20.96	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	41.92%#
11) 1,1-Dichloroethene-d2	2.095	63	243330	27.15	ug/L	-0.01
Spiked Amount	50.000	Range	60 - 125	Recovery	=	54.30%#
21) 2-Butanone-d5	3.825	46	454	0.19	ug/L	-0.07
Spiked Amount	100.000	Range	40 - 130	Recovery	=	0.19%#
24) Chloroform-d	4.349	84	350638	40.48	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	80.96%
26) 1,2-Dichloroethane-d4	5.034	65	269141	48.88	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.76%
32) Benzene-d6	5.047	84	623062	41.30	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	82.60%
36) 1,2-Dichloropropane-d6	6.072	67	179209	39.80	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	79.60%
41) Toluene-d8	7.320	98	611942	41.91	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	83.82%
43) trans-1,3-Dichloroprop...	7.629	79	108222	43.98	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	87.96%
47) 2-Hexanone-d5	8.127	63	141479	79.22	ug/L	0.04
Spiked Amount	100.000	Range	45 - 130	Recovery	=	79.22%
56) 1,1,2,2-Tetrachloroeth...	10.233	84	249319	36.71	ug/L	0.01
Spiked Amount	50.000	Range	65 - 120	Recovery	=	73.42%
66) 1,2-Dichlorobenzene-d4	11.635	152	299308	45.77	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	91.54%
Target Compounds						
68) 1,2-Dibromo-3-chloropr...	12.519	75	1412	0.84	ug/L	# 21


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042921\
Data File : VV021223.D
Acq On : 29 Apr 2021 16:17
Operator : SY/MD
Sample : M2177-05ME
Misc : 5.49g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Apr 30 05:57:20 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 30 05:55:34 2021
Response via : Initial Calibration

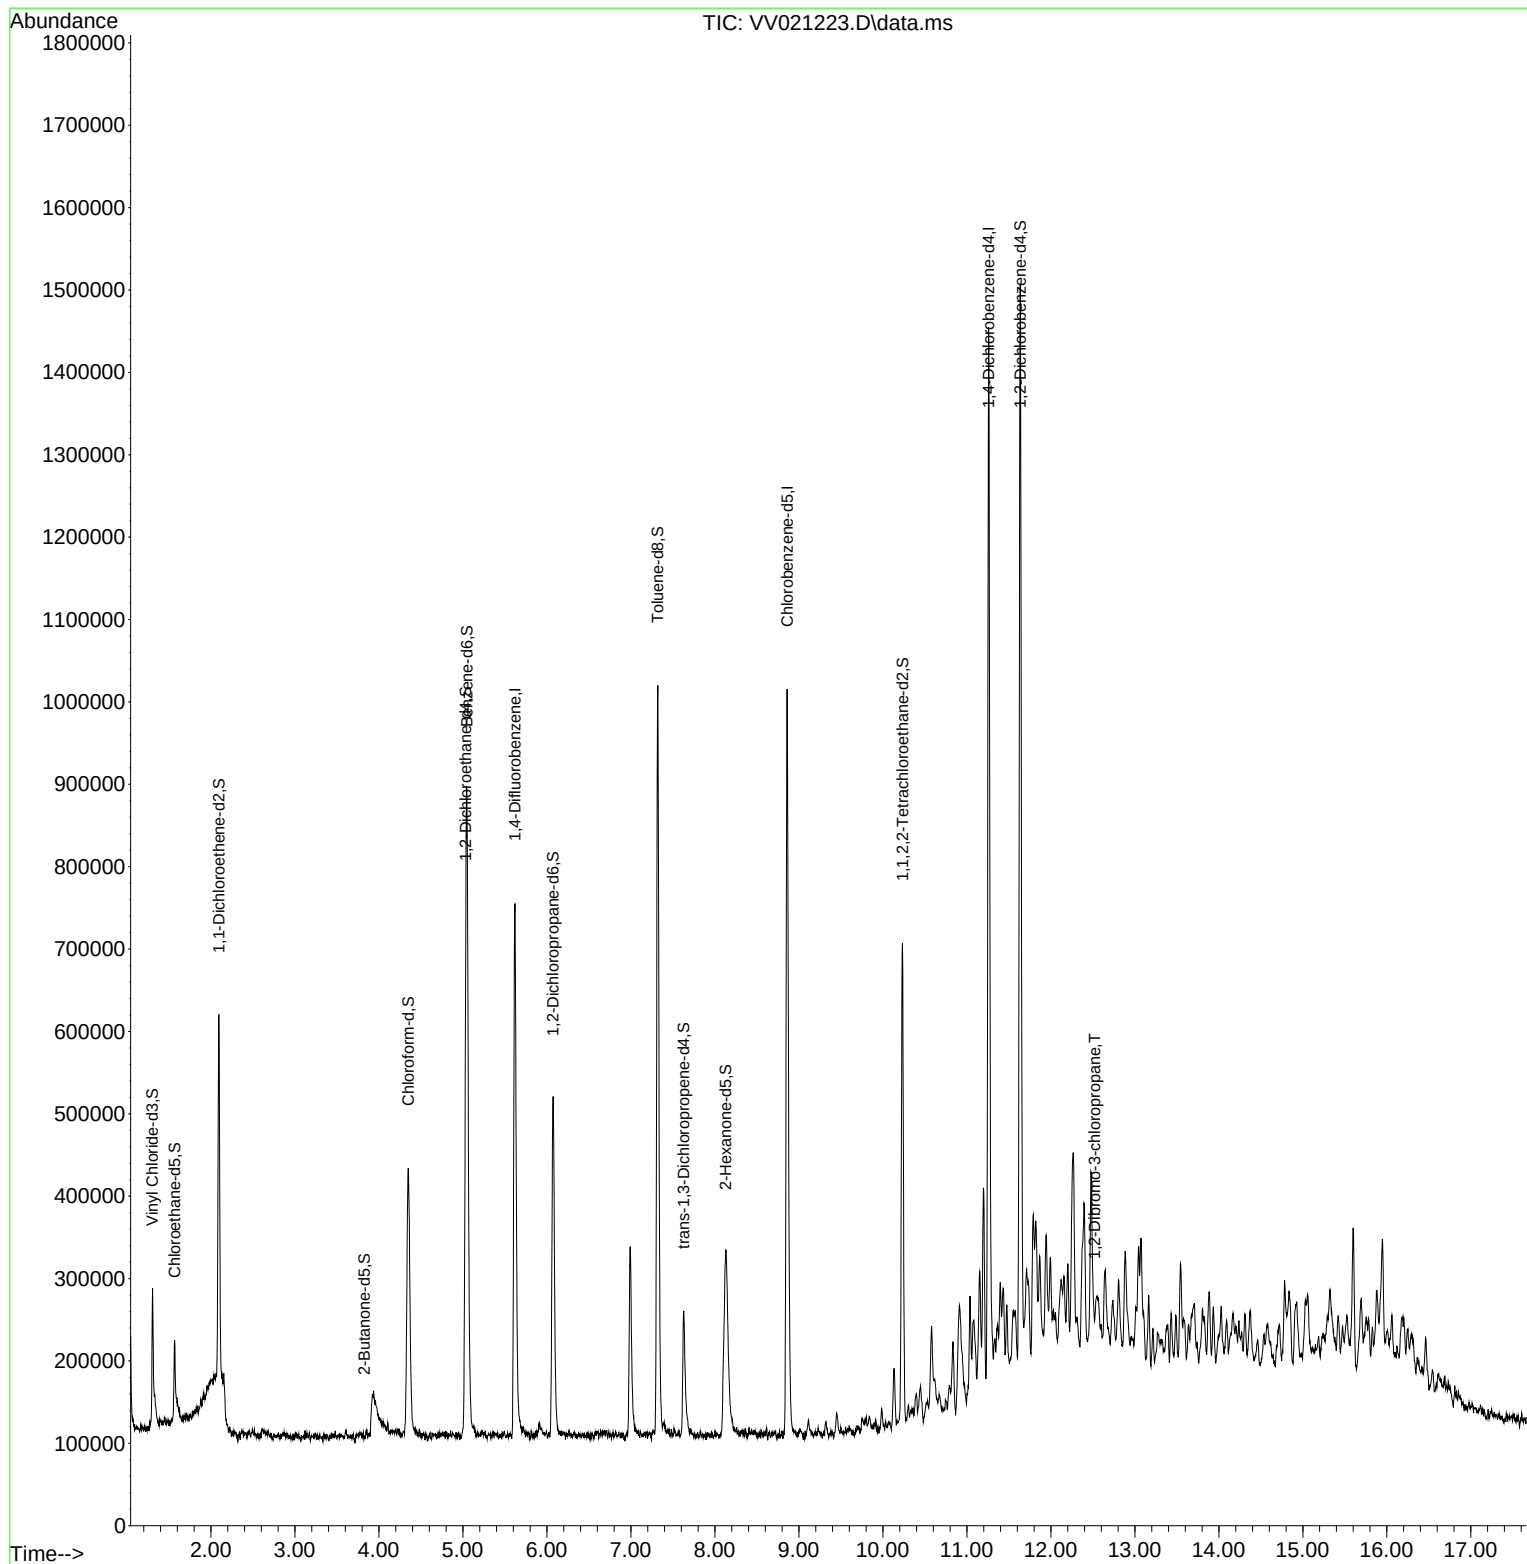

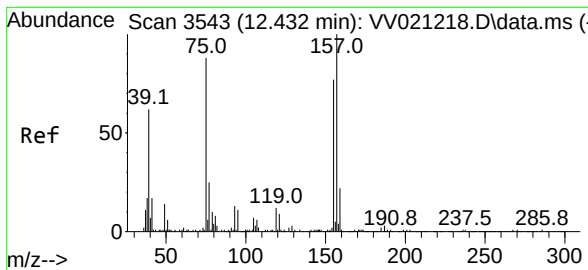

#68
 1,2-Dibromo-3-chloropropane
 Concen: 0.84 ug/L
 RT: 12.519 min Scan# 3570
 Delta R.T. 0.087 min
 Lab File: VV021223.D
 Acq: 29 Apr 2021 16:17

Instrument :
 MSVOA_V
 ClientSampleId :

Tgt Ion: 75 Resp: 1412
 Ion Ratio Lower Upper
 75 100
 155 28.0 72.8 109.2#
 157 20.0 94.6 142.0#

