

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
 Data File : VV035463.D
 Acq On : 29 Apr 2024 12:11
 Operator : SY/MD
 Sample : P2279-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RQ4

Quant Time: Apr 30 02:10:33 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 30 02:09:05 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	505277	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	504587	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	223458	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	171339	42.195	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	84.380%	
7) Chloroethane-d5	1.529	69	132433	56.922	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	113.840%	
11) 1,1-Dichloroethene-d2	2.053	65	73278	44.153	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	88.300%	
21) 2-Butanone-d5	3.799	46	221105	106.241	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	106.240%	
24) Chloroform-d	4.246	84	314507	46.028	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	92.060%	
26) 1,2-Dichloroethane-d4	4.937	65	196756	49.438	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	98.880%	
32) Benzene-d6	4.957	84	632181	47.675	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	95.360%	
36) 1,2-Dichloropropane-d6	5.985	67	201499	49.252	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	98.500%	
41) Toluene-d8	7.243	98	545505	45.642	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	91.280%	
43) trans-1,3-Dichloroprop...	7.551	79	88863	46.431	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	92.860%	
47) 2-Hexanone-d5	8.030	63	120505	102.172	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	102.170%	
56) 1,1,2,2-Tetrachloroeth...	10.152	84	287258	49.263	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	98.520%	
66) 1,2-Dichlorobenzene-d4	11.561	152	204232	52.239	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	104.480%	
Target Compounds						
					Qvalue	
51) Chlorobenzene	8.812	112	1473864	147.725	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
Data File : VV035463.D
Acq On : 29 Apr 2024 12:11
Operator : SY/MD
Sample : P2279-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RQ4

Quant Time: Apr 30 02:10:33 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Apr 30 02:09:05 2024
Response via : Initial Calibration

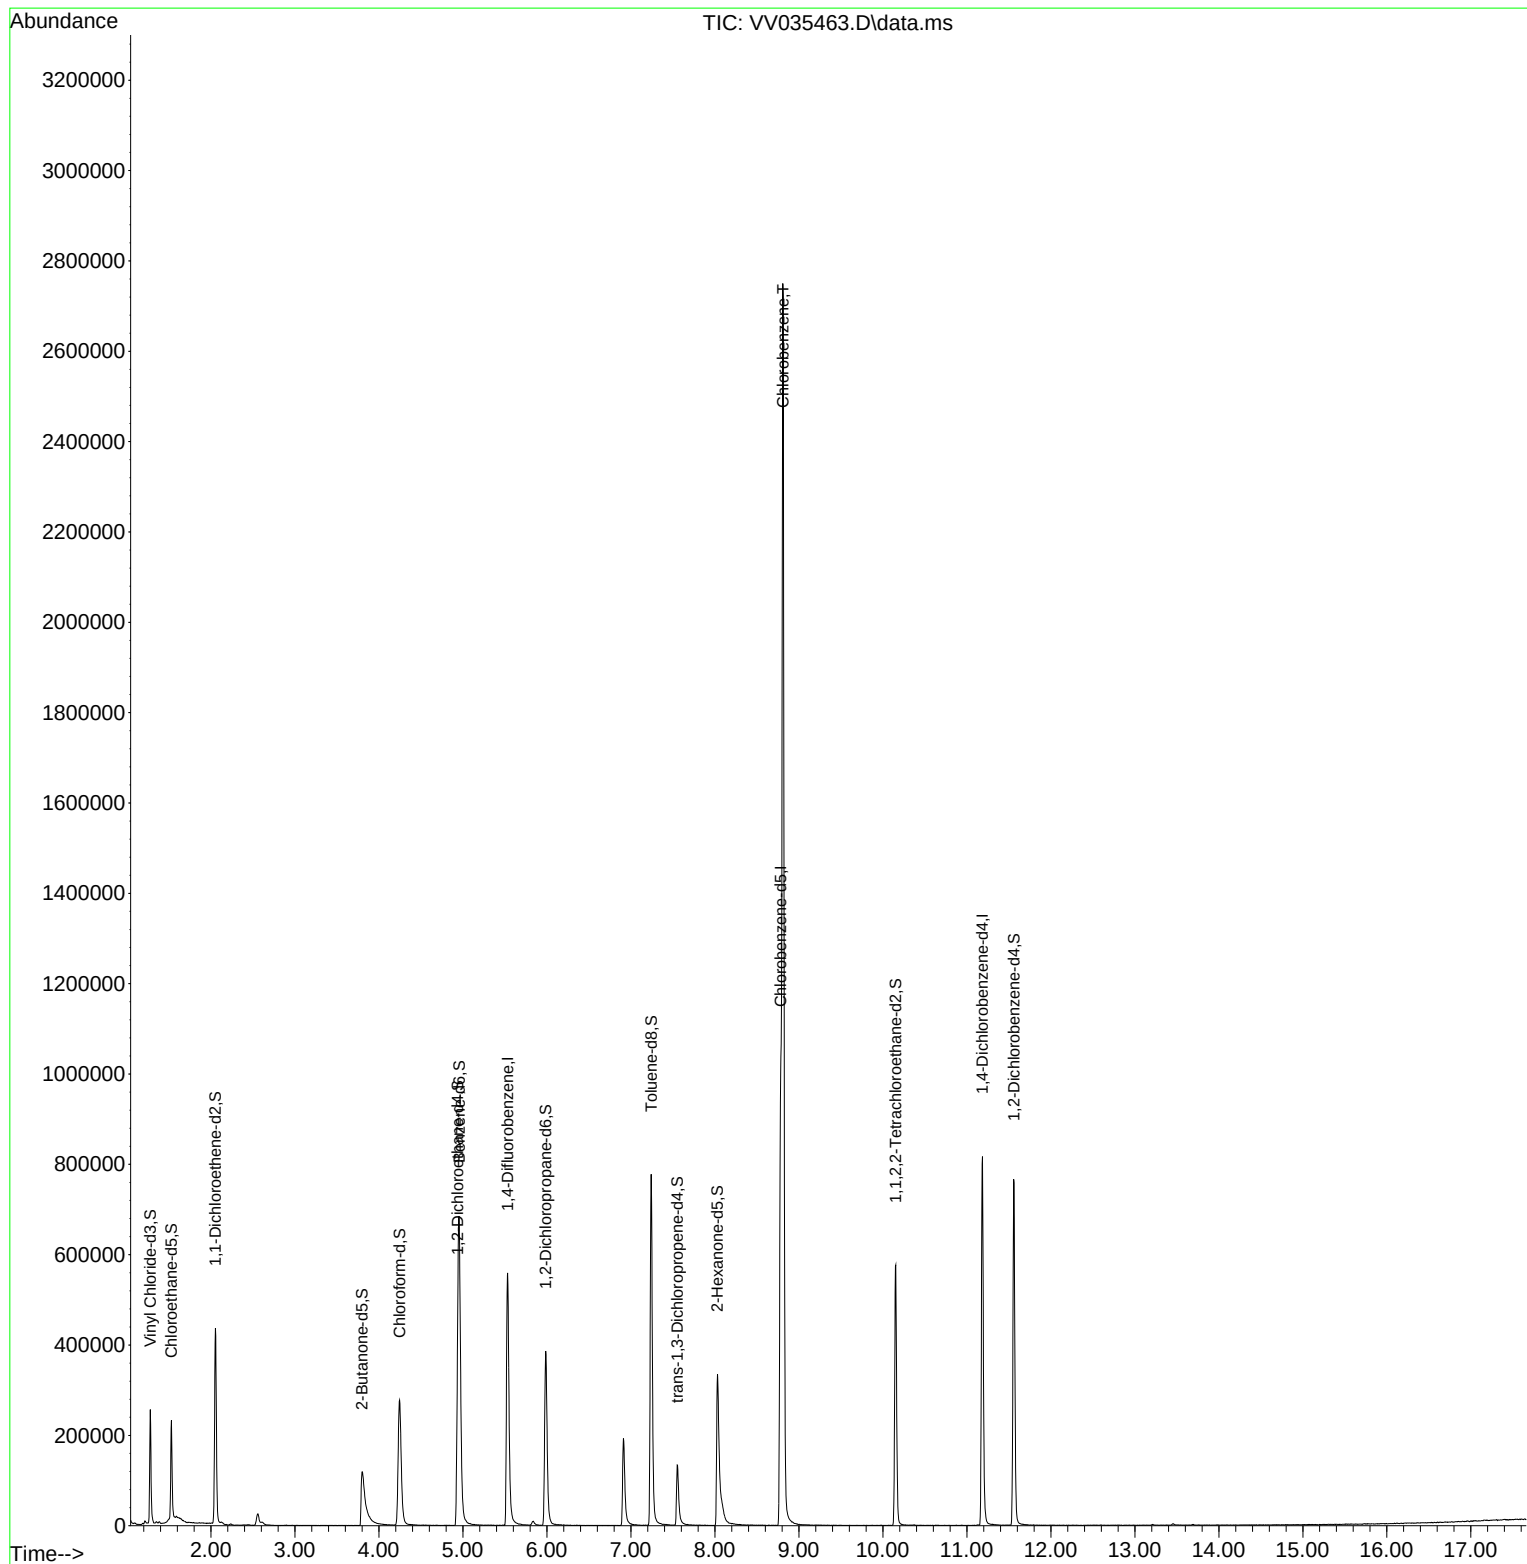

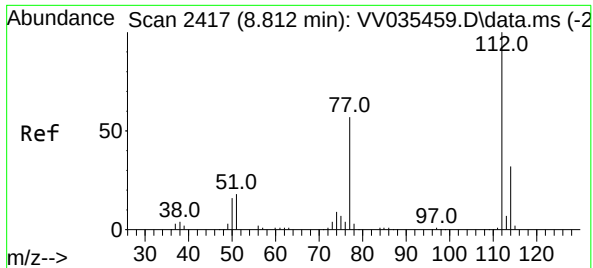

#51
Chlorobenzene
Concen: 147.725 ug/L
RT: 8.812 min Scan# 24
Delta R.T. -0.000 min
Lab File: VV035463.D
Acq: 29 Apr 2024 12:11

Instrument :
MSVOA_V
ClientSampleId :
C0RQ4

Tgt Ion:112 Resp: 1473864
Ion Ratio Lower Upper
112 100
114 32.8 22.4 41.6
77 58.2 45.6 68.4

