

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042924\
 Data File : VW035474.D
 Acq On : 29 Apr 2024 16:33
 Operator : SY/MD
 Sample : P2279-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORR3

Quant Time: Apr 30 02:13:29 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 30 02:09:05 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	521497	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	510983	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	217877	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	164364	39.218	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	78.440%		
7) Chloroethane-d5	1.529	69	132924	55.356	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	110.720%		
11) 1,1-Dichloroethene-d2	2.053	65	73529	42.926	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	85.860%		
21) 2-Butanone-d5	3.799	46	240559	111.994	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	111.990%		
24) Chloroform-d	4.246	84	321859	45.639	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	91.280%		
26) 1,2-Dichloroethane-d4	4.937	65	198246	48.263	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.520%		
32) Benzene-d6	4.957	84	628371	46.795	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.580%		
36) 1,2-Dichloropropane-d6	5.986	67	205255	49.542	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	99.080%		
41) Toluene-d8	7.243	98	534530	44.164	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	88.320%		
43) trans-1,3-Dichloroprop...	7.555	79	86600	44.682	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	89.360%		
47) 2-Hexanone-d5	8.030	63	129605	108.513	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	108.510%		
56) 1,1,2,2-Tetrachloroeth...	10.153	84	300954	50.965	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	101.940%		
66) 1,2-Dichlorobenzene-d4	11.558	152	202629	53.157	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	106.320%		
Target Compounds						Qvalue
3) Chloromethane	1.214	50	13182	3.388	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
Data File : VV035474.D
Acq On : 29 Apr 2024 16:33
Operator : SY/MD
Sample : P2279-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CORR3

Quant Time: Apr 30 02:13:29 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Apr 30 02:09:05 2024
Response via : Initial Calibration

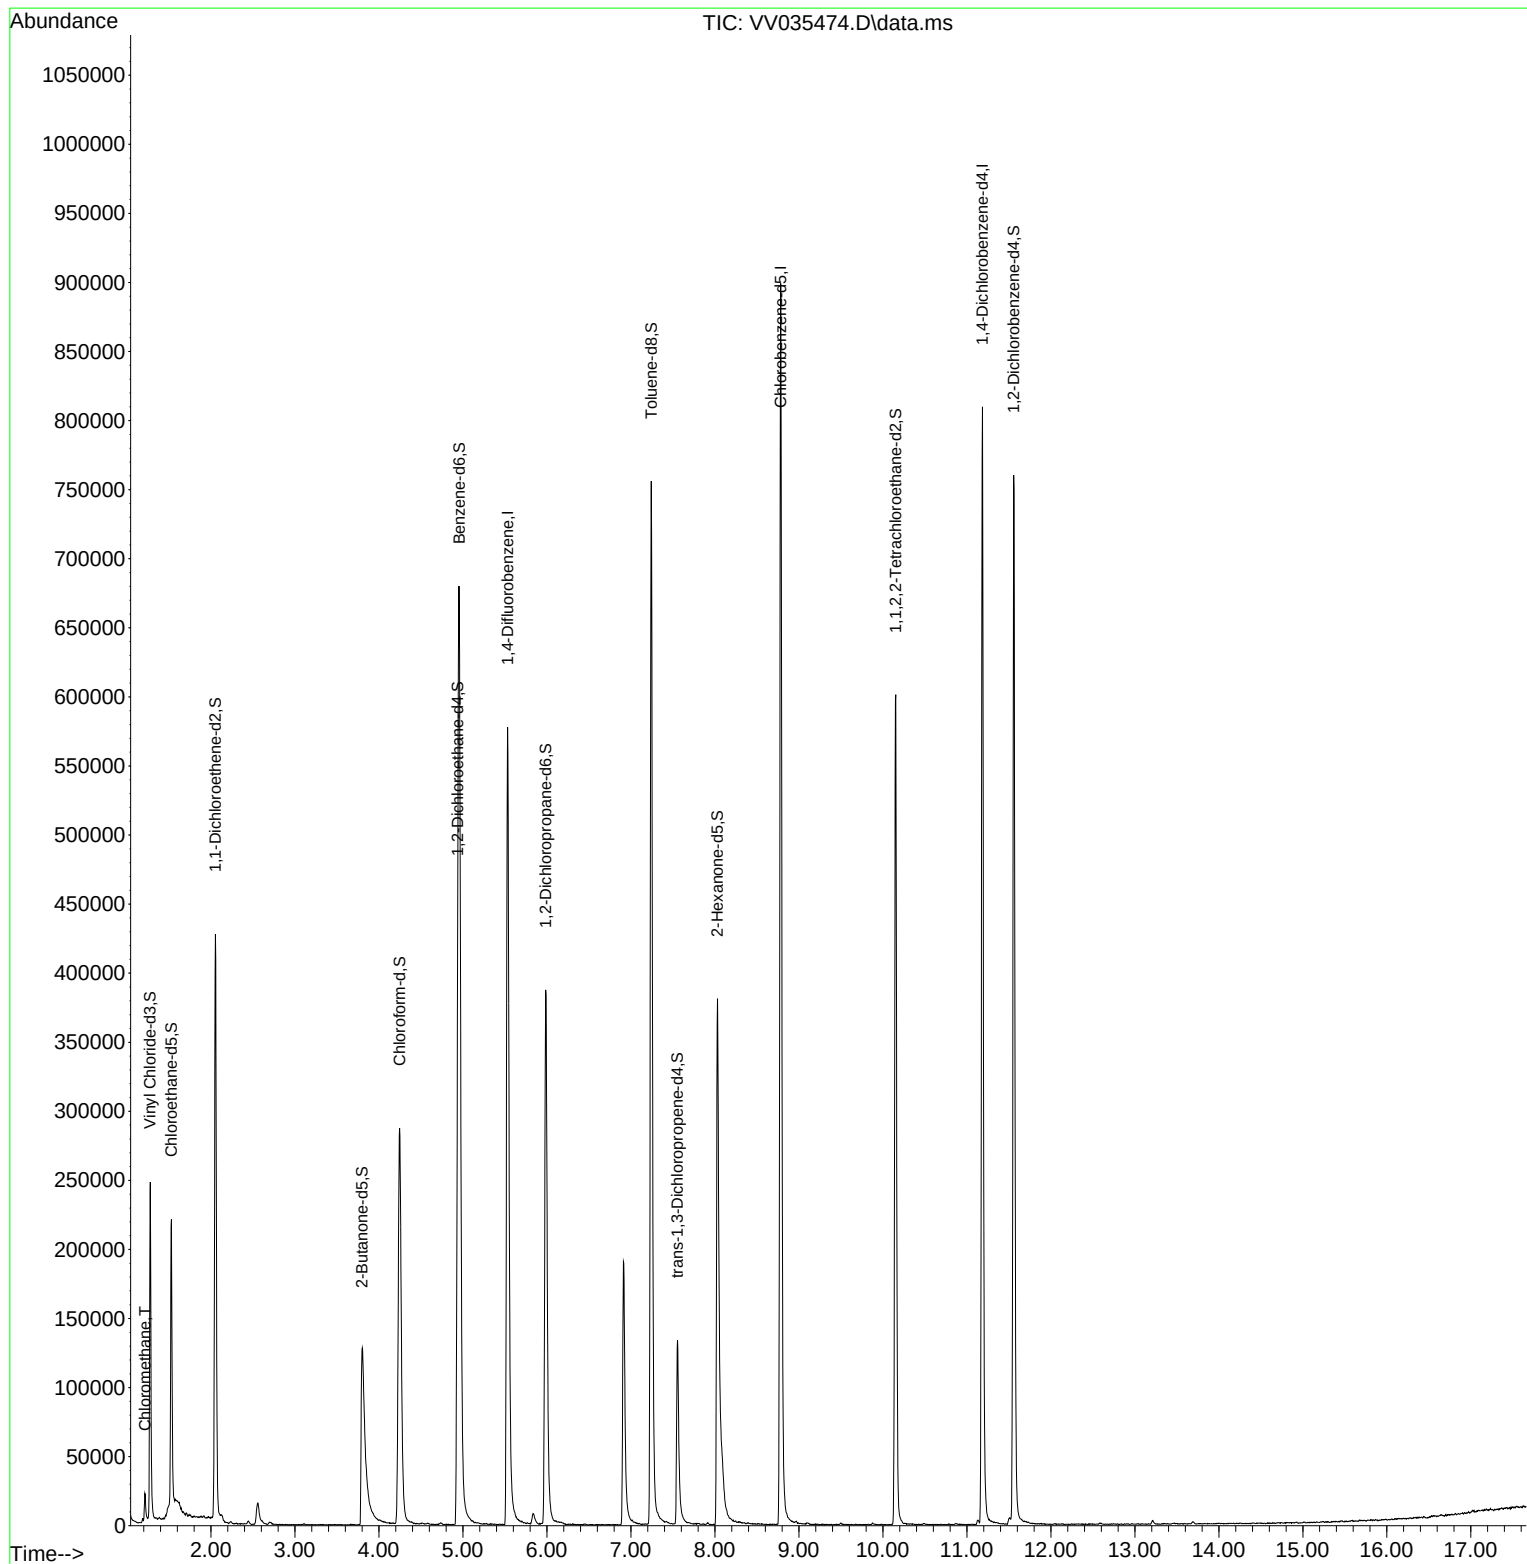

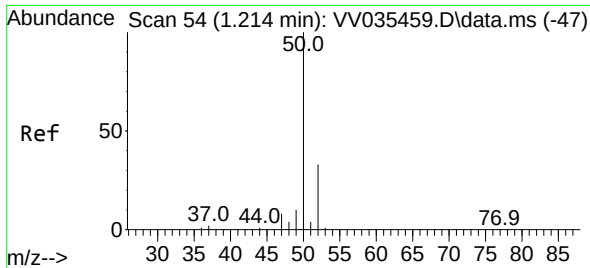

#3
 Chloromethane
 Concen: 3.388 ug/L
 RT: 1.214 min Scan# 54
 Delta R.T. 0.000 min
 Lab File: VV035474.D
 Acq: 29 Apr 2024 16:33

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RR3

Tgt Ion: 50 Resp: 13182
 Ion Ratio Lower Upper
 50 100
 52 34.0 23.0 42.8

