

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042924\
 Data File : VW035476.D
 Acq On : 29 Apr 2024 17:21
 Operator : SY/MD
 Sample : P2279-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORR7

Quant Time: Apr 30 02:13:58 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 30 02:09:05 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	360836	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	356272	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.184	152	148157	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	116535	40.186	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	80.380%		
7) Chloroethane-d5	1.529	69	96998	58.381	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	116.760%		
11) 1,1-Dichloroethene-d2	2.053	65	50278	42.421	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	84.840%		
21) 2-Butanone-d5	3.802	46	154505	103.958	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	103.960%		
24) Chloroform-d	4.249	84	220129	45.112	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	90.220%		
26) 1,2-Dichloroethane-d4	4.940	65	136692	48.094	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.180%		
32) Benzene-d6	4.956	84	426769	45.583	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	91.160%		
36) 1,2-Dichloropropane-d6	5.989	67	140162	48.521	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	97.040%		
41) Toluene-d8	7.243	98	351615	41.667	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	83.340%		
43) trans-1,3-Dichloroprop...	7.554	79	57348	42.438	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	84.880%		
47) 2-Hexanone-d5	8.030	63	78329	94.060	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	94.060%		
56) 1,1,2,2-Tetrachloroeth...	10.152	84	201888	49.035	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	98.080%		
66) 1,2-Dichlorobenzene-d4	11.561	152	134921	52.051	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	104.100%		
Target Compounds						Qvalue
3) Chloromethane	1.214	50	7367	2.737	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
Data File : VV035476.D
Acq On : 29 Apr 2024 17:21
Operator : SY/MD
Sample : P2279-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CORR7

Quant Time: Apr 30 02:13:58 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Apr 30 02:09:05 2024
Response via : Initial Calibration

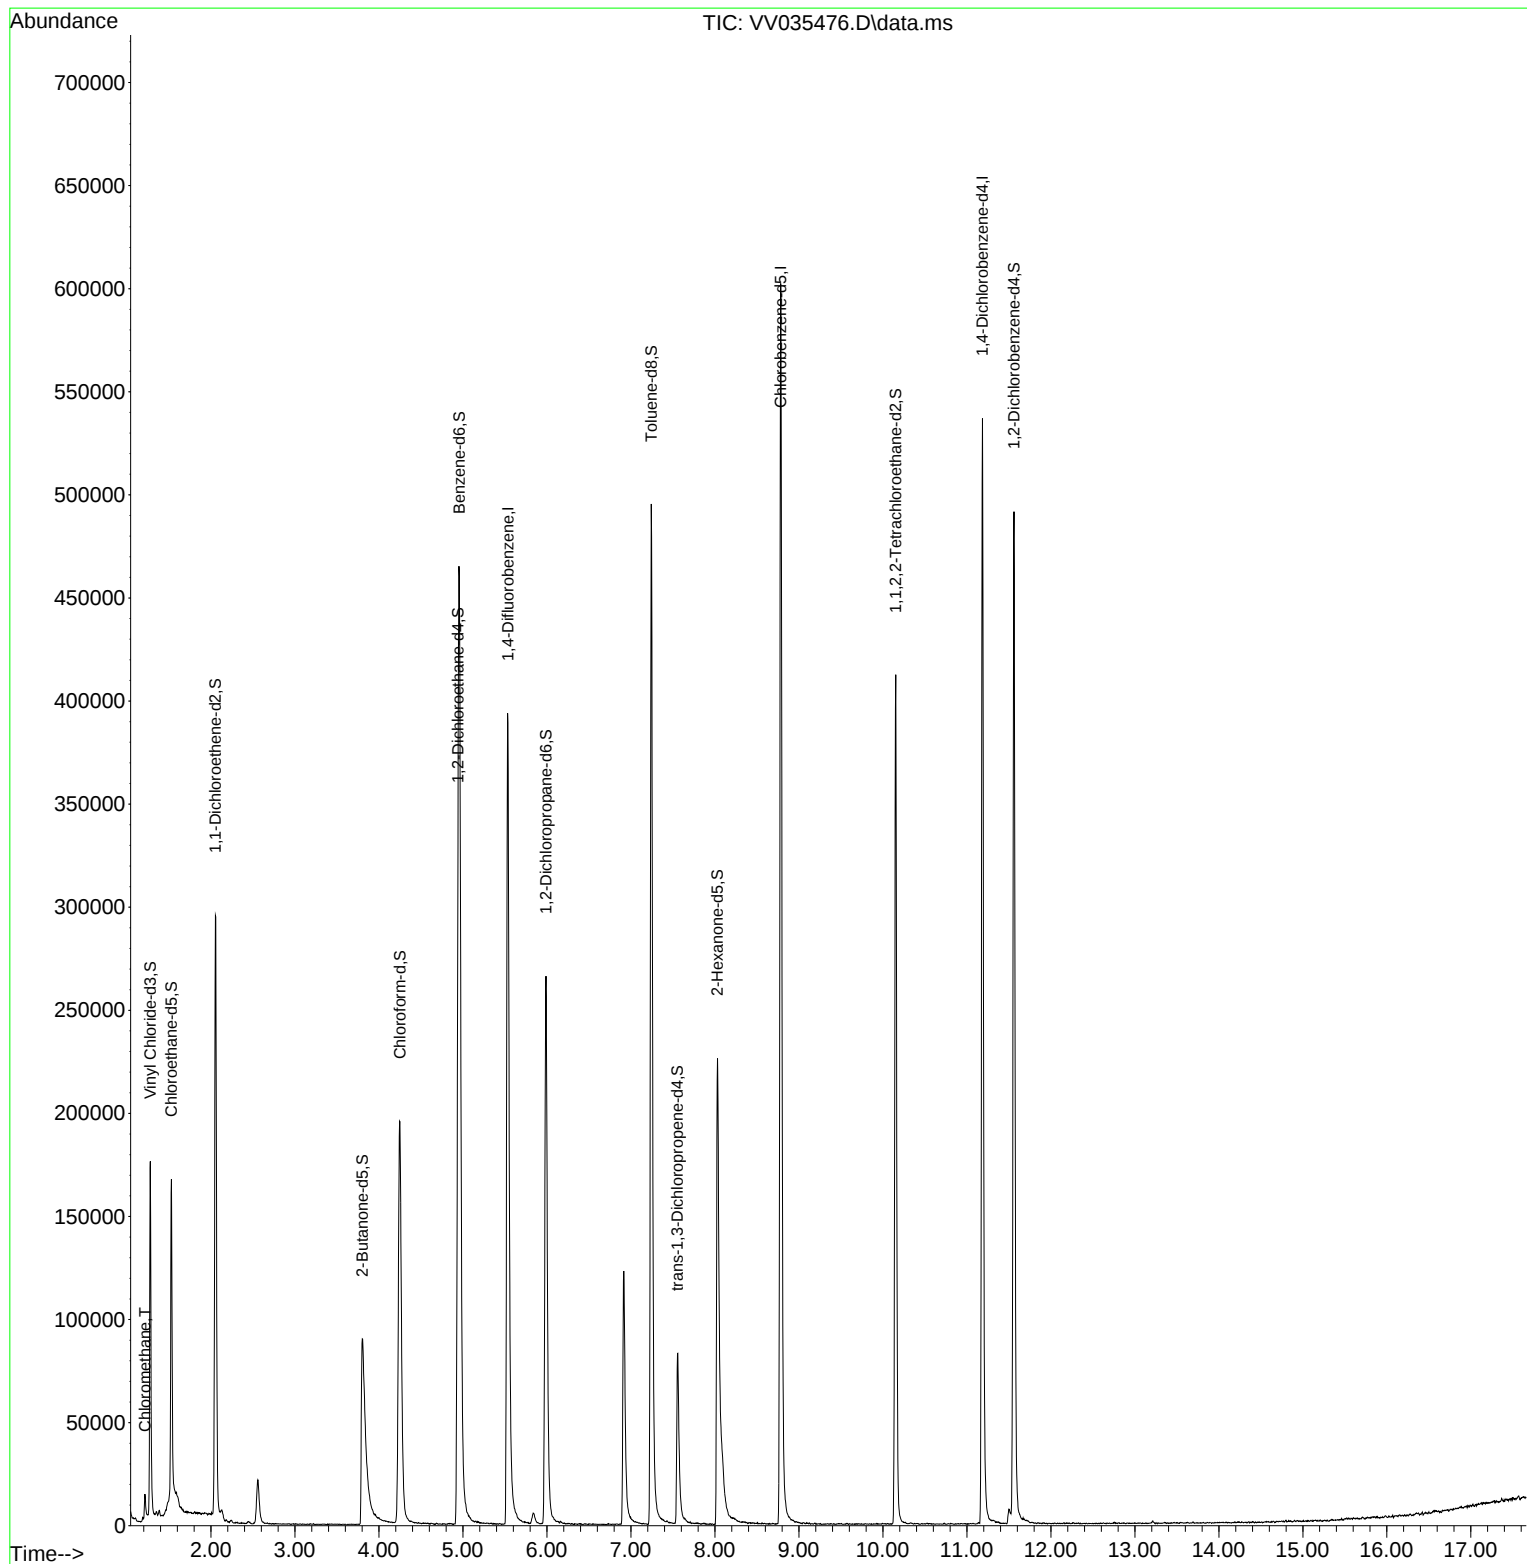

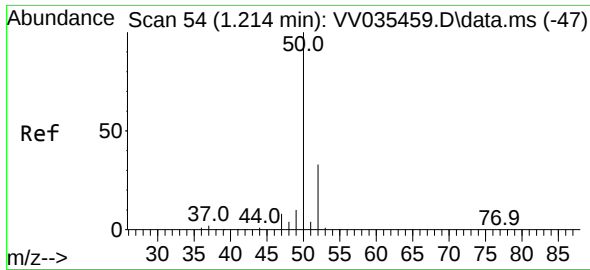

#3

Chloromethane

Concen: 2.737 ug/L

RT: 1.214 min Scan# 54

Delta R.T. -0.000 min

Lab File: VV035476.D


Acq: 29 Apr 2024 17:21

Instrument :

MSVOA_V

ClientSampleId :

C0RR7

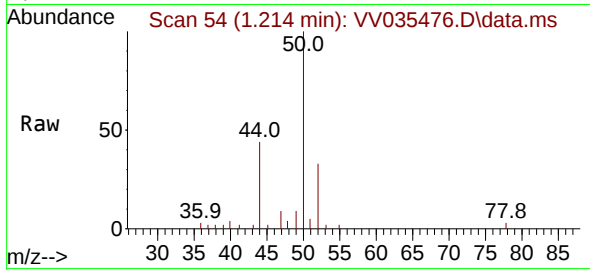

Tgt Ion: 50 Resp: 7367

Ion Ratio Lower Upper

50 100

52 33.0 23.0 42.8

