

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
 Data File : VV035460.D
 Acq On : 29 Apr 2024 10:39
 Operator : SY/MD
 Sample : VV0429WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK279

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035460.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.188	42	46	49	rBV	2129	1870	0.10%	0.013%
2	1.214	51	54	60	rVV4	2391	2750	0.14%	0.019%
3	1.278	67	74	90	rVB	267365	299171	15.60%	2.039%
4	1.529	145	152	164	rBV	215540	253098	13.19%	1.725%
5	2.053	304	315	331	rBV	463692	672339	35.05%	4.581%
6	2.442	432	436	445	rVB6	2057	2834	0.15%	0.019%
7	2.552	465	470	472	rBV2	790	707	0.04%	0.005%
8	2.619	488	491	495	rVB3	518	462	0.02%	0.003%
9	2.815	548	552	555	rBV2	391	376	0.02%	0.003%
10	2.973	598	601	603	rBV2	386	279	0.01%	0.002%
11	3.044	620	623	627	rVB2	439	394	0.02%	0.003%
12	3.085	633	636	642	rBV2	233	235	0.01%	0.002%
13	3.220	675	678	682	rVB2	289	221	0.01%	0.002%
14	3.574	786	788	794	rVB2	336	267	0.01%	0.002%
15	3.600	794	796	801	rBV	248	205	0.01%	0.001%
16	3.677	816	820	824	rBV2	345	317	0.02%	0.002%
17	3.802	850	859	906	rBV	120363	424659	22.14%	2.894%
18	4.153	965	968	973	rBV3	490	452	0.02%	0.003%
19	4.243	980	996	1033	rBV	299168	773788	40.34%	5.272%
20	4.523	1081	1083	1090	rVB4	523	370	0.02%	0.003%
21	4.651	1120	1123	1127	rVB	399	330	0.02%	0.002%
22	4.674	1127	1130	1135	rBV3	235	250	0.01%	0.002%
23	4.847	1181	1184	1187	rVB3	393	240	0.01%	0.002%
24	4.950	1197	1216	1254	rBV2	733275	1918167	100.00%	13.070%
25	5.310	1325	1328	1330	rVB2	458	254	0.01%	0.002%
26	5.342	1335	1338	1340	rVB	656	358	0.02%	0.002%
27	5.429	1362	1365	1370	rVB3	380	206	0.01%	0.001%
28	5.532	1385	1397	1435	rBV	576464	1216236	63.41%	8.287%
29	5.834	1480	1491	1507	rBV5	9038	21813	1.14%	0.149%
30	5.986	1524	1538	1569	rBV	405937	854759	44.56%	5.824%
31	6.268	1624	1626	1629	rBV3	390	271	0.01%	0.002%
32	6.285	1629	1631	1636	rVB2	696	525	0.03%	0.004%
33	6.365	1653	1656	1658	rBV3	393	282	0.01%	0.002%
34	6.378	1658	1660	1662	rVV	397	209	0.01%	0.001%
35	6.436	1673	1678	1682	rVB2	470	405	0.02%	0.003%
36	6.465	1685	1687	1690	rVB2	467	205	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
 Data File : VV035460.D
 Acq On : 29 Apr 2024 10:39
 Operator : SY/MD
 Sample : VV0429WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK279

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

37	6.487	1690	1694	1698	rVB3	448	376	0.02%	0.003%
38	6.574	1715	1721	1724	rBV2	403	259	0.01%	0.002%
39	6.912	1815	1826	1860	rBV	210786	411198	21.44%	2.802%
40	7.240	1917	1928	1966	rVV	833810	1477905	77.05%	10.070%
41	7.551	2016	2025	2053	rBV	147323	275988	14.39%	1.881%
42	7.760	2088	2090	2093	rBV2	546	283	0.01%	0.002%
43	7.825	2108	2110	2113	rVB2	408	214	0.01%	0.001%
44	7.947	2145	2148	2152	rVB2	360	291	0.02%	0.002%
45	7.976	2155	2157	2160	rBV2	315	238	0.01%	0.002%
46	8.034	2164	2175	2224	rBV2	359151	898491	46.84%	6.122%
47	8.468	2307	2310	2313	rBV2	555	375	0.02%	0.003%
48	8.484	2313	2315	2318	rVB4	366	214	0.01%	0.001%
49	8.510	2319	2323	2325	rBV2	455	321	0.02%	0.002%
50	8.558	2336	2338	2341	rVV3	731	520	0.03%	0.004%
51	8.574	2341	2343	2348	rVB2	637	391	0.02%	0.003%
52	8.702	2381	2383	2386	rBV2	427	238	0.01%	0.002%
53	8.783	2396	2408	2441	rBV	888086	1486727	77.51%	10.130%
54	9.014	2478	2480	2483	rBV3	645	489	0.03%	0.003%
55	9.188	2533	2534	2540	rBV2	247	228	0.01%	0.002%
56	9.493	2623	2629	2632	rBV3	499	444	0.02%	0.003%
57	9.519	2635	2637	2642	rBV3	281	218	0.01%	0.001%
58	9.702	2691	2694	2697	rVB2	471	303	0.02%	0.002%
59	9.876	2740	2748	2757	rBV5	617	1187	0.06%	0.008%
60	9.973	2774	2778	2780	rBV2	304	267	0.01%	0.002%
61	10.034	2792	2797	2800	rBV2	245	204	0.01%	0.001%
62	10.104	2817	2819	2822	rBV	287	238	0.01%	0.002%
63	10.153	2822	2834	2860	rBV	621503	991488	51.69%	6.756%
64	10.355	2894	2897	2901	rVB3	338	235	0.01%	0.002%
65	10.429	2917	2920	2928	rVB3	448	564	0.03%	0.004%
66	10.484	2932	2937	2938	rBV2	607	412	0.02%	0.003%
67	10.590	2968	2970	2975	rVB2	326	230	0.01%	0.002%
68	10.664	2990	2993	3002	rVB2	299	357	0.02%	0.002%
69	10.767	3022	3025	3028	rBV2	428	262	0.01%	0.002%
70	10.786	3028	3031	3035	rVB3	380	321	0.02%	0.002%
71	10.837	3043	3047	3049	rBV	428	282	0.01%	0.002%
72	10.870	3050	3057	3064	rVB5	915	1409	0.07%	0.010%
73	10.908	3064	3069	3074	rBV3	370	533	0.03%	0.004%
74	11.130	3132	3138	3144	rBV4	1750	2525	0.13%	0.017%
75	11.185	3144	3155	3184	rBV	828138	1307747	68.18%	8.911%
76	11.503	3247	3254	3256	rBV3	677	691	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
 Data File : VV035460.D
 Acq On : 29 Apr 2024 10:39
 Operator : SY/MD
 Sample : VV0429WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK279

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

77	11.558	3259	3271	3295	rBV	807386	1274277	66.43%	8.683%
78	11.844	3358	3360	3363	rVB2	510	258	0.01%	0.002%
79	11.886	3370	3373	3375	rBV	378	229	0.01%	0.002%
80	11.918	3380	3383	3385	rBV	452	259	0.01%	0.002%
81	12.159	3454	3458	3461	rBV3	471	457	0.02%	0.003%
82	12.297	3498	3501	3507	rVB2	322	257	0.01%	0.002%
83	12.381	3522	3527	3530	rVB6	390	447	0.02%	0.003%
84	12.590	3587	3592	3604	rBV8	2491	3975	0.21%	0.027%
85	12.667	3614	3616	3620	rVB2	523	294	0.02%	0.002%
86	12.712	3625	3630	3634	rBV4	462	492	0.03%	0.003%
87	12.821	3659	3664	3666	rBV2	307	246	0.01%	0.002%
88	12.847	3670	3672	3677	rVV3	389	311	0.02%	0.002%
89	12.947	3701	3703	3706	rVB2	385	211	0.01%	0.001%
90	13.069	3737	3741	3744	rBV2	267	257	0.01%	0.002%
91	13.207	3776	3784	3799	rVB5	6241	11080	0.58%	0.075%
92	13.313	3814	3817	3820	rBV	359	224	0.01%	0.002%
93	13.445	3848	3858	3874	rBV	29699	52005	2.71%	0.354%
94	13.683	3924	3932	3948	rVB4	8166	13825	0.72%	0.094%
95	13.911	3998	4003	4007	rBV2	602	645	0.03%	0.004%
96	14.191	4087	4090	4094	rBV4	548	362	0.02%	0.002%
97	14.496	4183	4185	4189	rVB2	589	315	0.02%	0.002%
98	14.561	4203	4205	4209	rBV2	450	290	0.02%	0.002%
99	14.718	4252	4254	4262	rVB5	845	991	0.05%	0.007%
100	14.770	4268	4270	4272	rBV	596	265	0.01%	0.002%




Sum of corrected areas: 14675939

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
Data File : VV035460.D
Acq On : 29 Apr 2024 10:39
Operator : SY/MD
Sample : VV0429WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK279

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

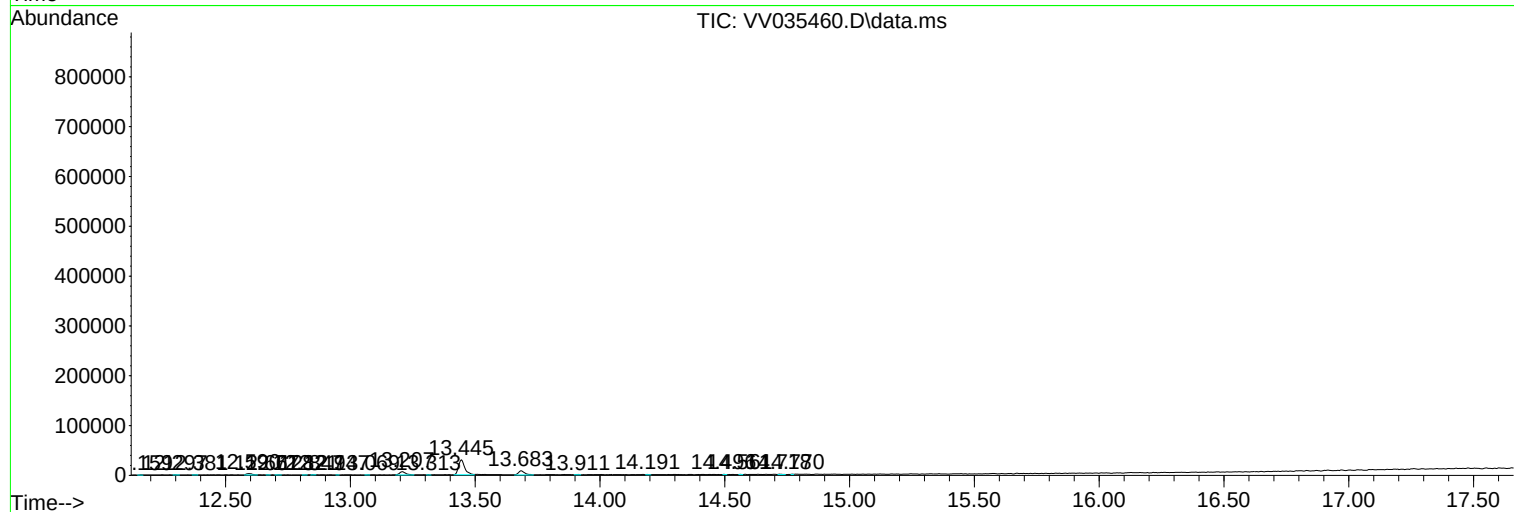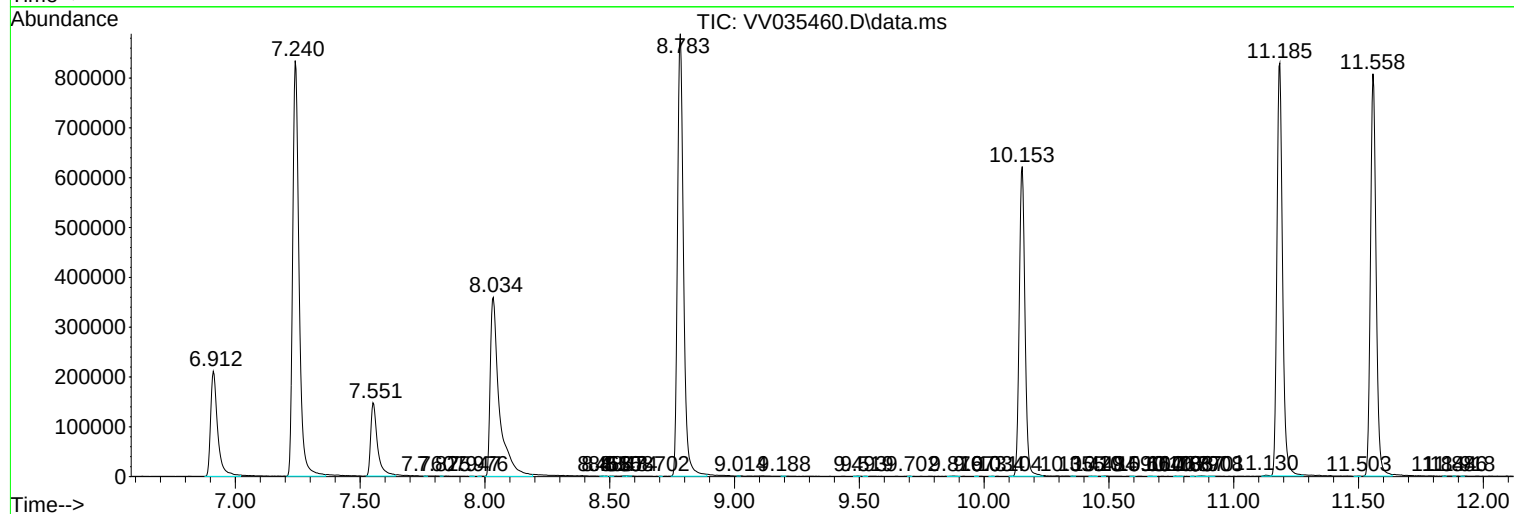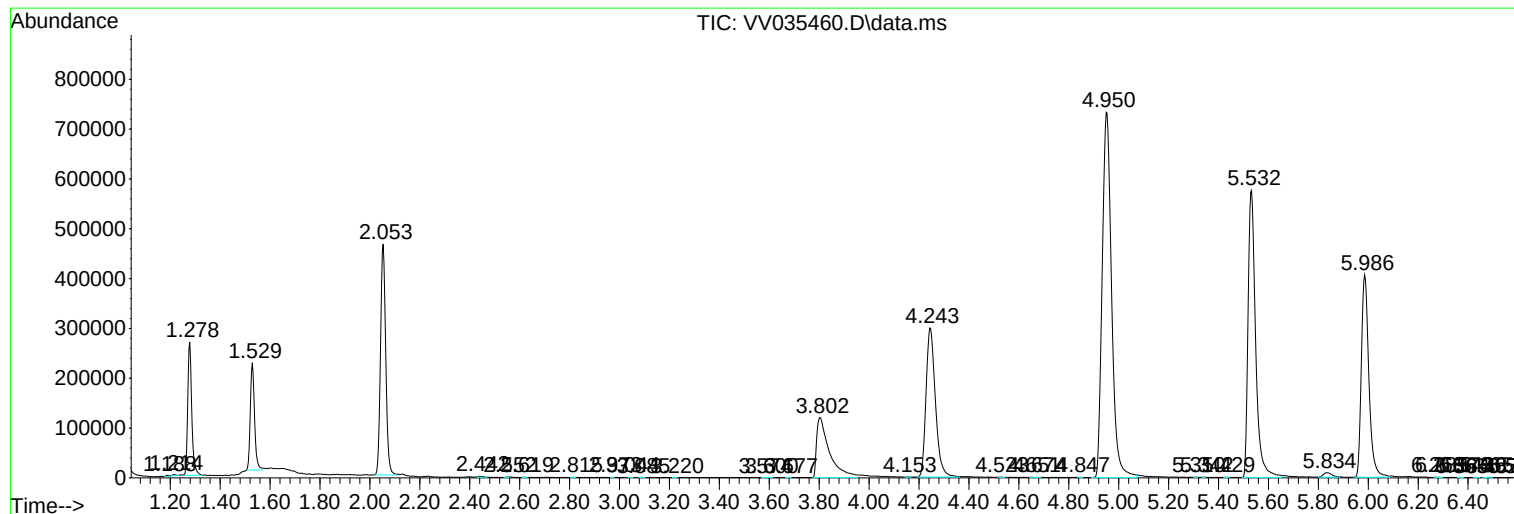

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
Data File : VV035460.D
Acq On : 29 Apr 2024 10:39
Operator : SY/MD
Sample : VV0429WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK279

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
Data File : VV035460.D
Acq On : 29 Apr 2024 10:39
Operator : SY/MD
Sample : VV0429WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK279

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------