

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
 Data File : VV035462.D
 Acq On : 29 Apr 2024 11:47
 Operator : SY/MD
 Sample : P2204-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035462.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.188	42	46	49	rBV	2394	1995	0.11%	0.014%
2	1.214	50	54	57	rBV4	3353	2839	0.15%	0.020%
3	1.278	67	74	93	rVB	249884	278076	15.01%	1.974%
4	1.529	145	152	165	rBV	220666	263763	14.24%	1.873%
5	2.053	305	315	331	rBV	437074	629473	33.97%	4.469%
6	2.310	393	395	399	rVB3	517	379	0.02%	0.003%
7	2.387	417	419	426	rBV5	632	738	0.04%	0.005%
8	2.445	431	437	447	rVB5	2676	4140	0.22%	0.029%
9	2.696	511	515	519	rVV3	447	408	0.02%	0.003%
10	2.825	552	555	559	rVV3	291	193	0.01%	0.001%
11	3.024	615	617	624	rBV3	371	303	0.02%	0.002%
12	3.063	625	629	634	rBV2	246	222	0.01%	0.002%
13	3.223	675	679	683	rVB2	220	216	0.01%	0.002%
14	3.336	710	714	717	rVV2	290	197	0.01%	0.001%
15	3.567	782	786	790	rVB2	387	322	0.02%	0.002%
16	3.735	831	838	842	rBV2	322	439	0.02%	0.003%
17	3.802	850	859	922	rBV	122082	447658	24.16%	3.178%
18	4.246	981	997	1038	rBV	288129	744986	40.21%	5.289%
19	4.497	1073	1075	1079	rVB3	474	248	0.01%	0.002%
20	4.609	1108	1110	1116	rBV2	244	282	0.02%	0.002%
21	4.747	1151	1153	1157	rVB2	496	296	0.02%	0.002%
22	4.834	1172	1180	1181	rBV3	306	399	0.02%	0.003%
23	4.953	1201	1217	1252	rBV2	705094	1852864	100.00%	13.155%
24	5.239	1305	1306	1310	rBV4	329	198	0.01%	0.001%
25	5.329	1330	1334	1335	rBV	509	328	0.02%	0.002%
26	5.532	1385	1397	1433	rBV	531768	1122565	60.59%	7.970%
27	5.831	1480	1490	1509	rBV3	8958	20994	1.13%	0.149%
28	5.985	1523	1538	1569	rBV	402893	842379	45.46%	5.981%
29	6.342	1645	1649	1650	rBV3	630	420	0.02%	0.003%
30	6.403	1664	1668	1671	rVB2	265	211	0.01%	0.001%
31	6.448	1681	1682	1688	rVB3	354	199	0.01%	0.001%
32	6.503	1696	1699	1702	rBV2	426	324	0.02%	0.002%
33	6.554	1713	1715	1722	rVB2	366	283	0.02%	0.002%
34	6.735	1766	1771	1776	rVB2	333	295	0.02%	0.002%
35	6.911	1815	1826	1859	rBV	203682	398049	21.48%	2.826%
36	7.130	1892	1894	1897	rBV3	482	244	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
 Data File : VV035462.D
 Acq On : 29 Apr 2024 11:47
 Operator : SY/MD
 Sample : P2204-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

37	7.243	1917	1929	1958	rBV	794907	1416582	76.45%	10.057%
38	7.551	2015	2025	2050	rBV	141913	268234	14.48%	1.904%
39	7.834	2111	2113	2118	rBV4	266	214	0.01%	0.002%
40	7.886	2125	2129	2133	rBV4	577	417	0.02%	0.003%
41	7.918	2136	2139	2143	rBV3	432	230	0.01%	0.002%
42	7.969	2151	2155	2157	rVB3	656	370	0.02%	0.003%
43	8.033	2165	2175	2224	rBV2	367206	907302	48.97%	6.442%
44	8.522	2324	2327	2330	rBV3	313	193	0.01%	0.001%
45	8.561	2334	2339	2343	rBV4	663	819	0.04%	0.006%
46	8.660	2367	2370	2372	rVV	367	243	0.01%	0.002%
47	8.673	2372	2374	2378	rVB	469	275	0.01%	0.002%
48	8.783	2397	2408	2437	rBV	833109	1377792	74.36%	9.782%
49	9.017	2479	2481	2483	rBV	514	262	0.01%	0.002%
50	9.075	2496	2499	2500	rBV2	532	291	0.02%	0.002%
51	9.140	2513	2519	2522	rBV2	303	330	0.02%	0.002%
52	9.204	2537	2539	2545	rBV2	322	270	0.01%	0.002%
53	9.271	2556	2560	2564	rBV2	364	240	0.01%	0.002%
54	9.358	2584	2587	2590	rVB2	532	295	0.02%	0.002%
55	9.574	2652	2654	2658	rVB	418	266	0.01%	0.002%
56	9.648	2673	2677	2686	rVB	470	567	0.03%	0.004%
57	9.886	2748	2751	2754	rVB2	489	280	0.02%	0.002%
58	9.908	2754	2758	2763	rBV2	403	386	0.02%	0.003%
59	9.956	2771	2773	2779	rVB	366	283	0.02%	0.002%
60	10.030	2794	2796	2803	rBV2	249	227	0.01%	0.002%
61	10.152	2822	2834	2864	rBV	624850	996836	53.80%	7.077%
62	10.358	2894	2898	2900	rBV2	324	258	0.01%	0.002%
63	10.493	2938	2940	2943	rVB	375	208	0.01%	0.001%
64	10.860	3051	3054	3055	rBV	368	212	0.01%	0.002%
65	10.898	3063	3066	3070	rVB2	340	255	0.01%	0.002%
66	11.130	3135	3138	3139	rBV2	553	281	0.02%	0.002%
67	11.184	3144	3155	3187	rBV	776085	1224046	66.06%	8.690%
68	11.487	3246	3249	3253	rBV3	602	487	0.03%	0.003%
69	11.512	3255	3257	3260	rBV3	343	214	0.01%	0.002%
70	11.557	3260	3271	3299	rBV	776979	1245845	67.24%	8.845%
71	11.869	3366	3368	3370	rBV2	381	193	0.01%	0.001%
72	11.934	3385	3388	3392	rBV2	427	404	0.02%	0.003%
73	12.020	3411	3415	3419	rBV3	387	261	0.01%	0.002%
74	12.069	3427	3430	3432	rBV2	377	240	0.01%	0.002%
75	12.168	3458	3461	3466	rVB	341	273	0.01%	0.002%
76	12.291	3496	3499	3501	rVB2	398	222	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
 Data File : VV035462.D
 Acq On : 29 Apr 2024 11:47
 Operator : SY/MD
 Sample : P2204-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

77	12.390	3526	3530	3533	rBV3	426	344	0.02%	0.002%
78	12.410	3533	3536	3539	rVB3	413	266	0.01%	0.002%
79	12.435	3539	3544	3546	rBV2	335	284	0.02%	0.002%
80	12.458	3549	3551	3555	rVB2	420	279	0.02%	0.002%
81	12.596	3588	3594	3601	rBV3	910	1211	0.07%	0.009%
82	12.625	3601	3603	3606	rVV4	433	288	0.02%	0.002%
83	12.647	3608	3610	3614	rVV2	484	332	0.02%	0.002%
84	12.670	3614	3617	3623	rVB3	522	450	0.02%	0.003%
85	12.705	3623	3628	3634	rBV2	384	479	0.03%	0.003%
86	12.737	3634	3638	3641	rBV3	504	325	0.02%	0.002%
87	12.930	3695	3698	3701	rBV2	501	337	0.02%	0.002%
88	12.975	3707	3712	3716	rBV3	463	520	0.03%	0.004%
89	13.168	3769	3772	3776	rVB2	576	394	0.02%	0.003%
90	13.210	3776	3785	3794	rBV8	1990	3604	0.19%	0.026%
91	13.245	3794	3796	3800	rVB3	546	306	0.02%	0.002%
92	13.323	3817	3820	3823	rVB2	404	216	0.01%	0.002%
93	13.451	3854	3860	3871	rBV3	4450	7202	0.39%	0.051%
94	13.557	3889	3893	3894	rBV2	364	224	0.01%	0.002%
95	13.689	3927	3934	3946	rBV4	1764	2635	0.14%	0.019%
96	13.979	4021	4024	4029	rVB2	709	493	0.03%	0.004%
97	14.152	4076	4078	4080	rBV	388	234	0.01%	0.002%
98	14.233	4101	4103	4106	rBV2	473	246	0.01%	0.002%
99	14.737	4258	4260	4262	rBV2	658	391	0.02%	0.003%
100	14.959	4327	4329	4331	rBV	721	422	0.02%	0.003%




Sum of corrected areas: 14085010

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
Data File : VV035462.D
Acq On : 29 Apr 2024 11:47
Operator : SY/MD
Sample : P2204-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

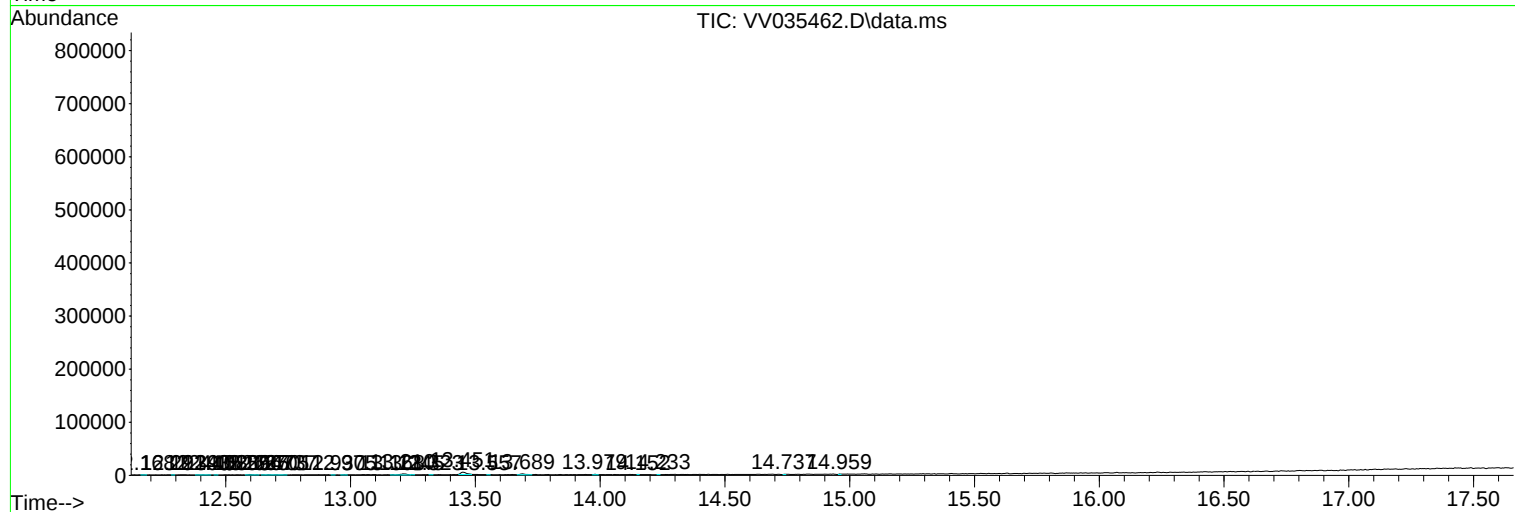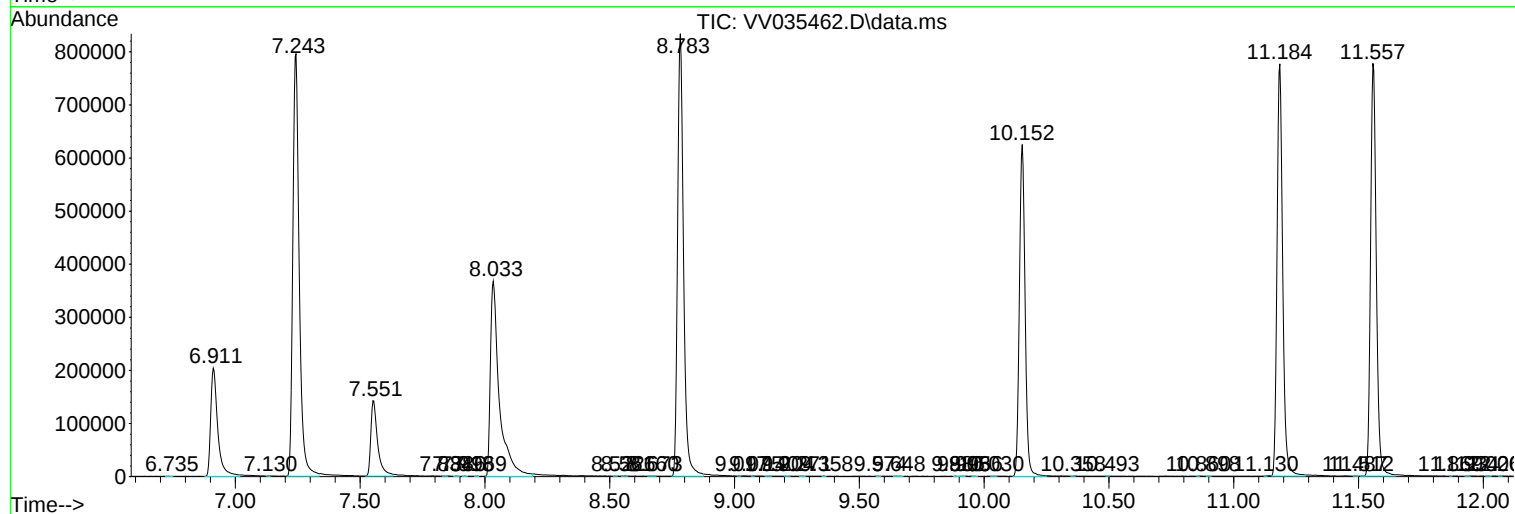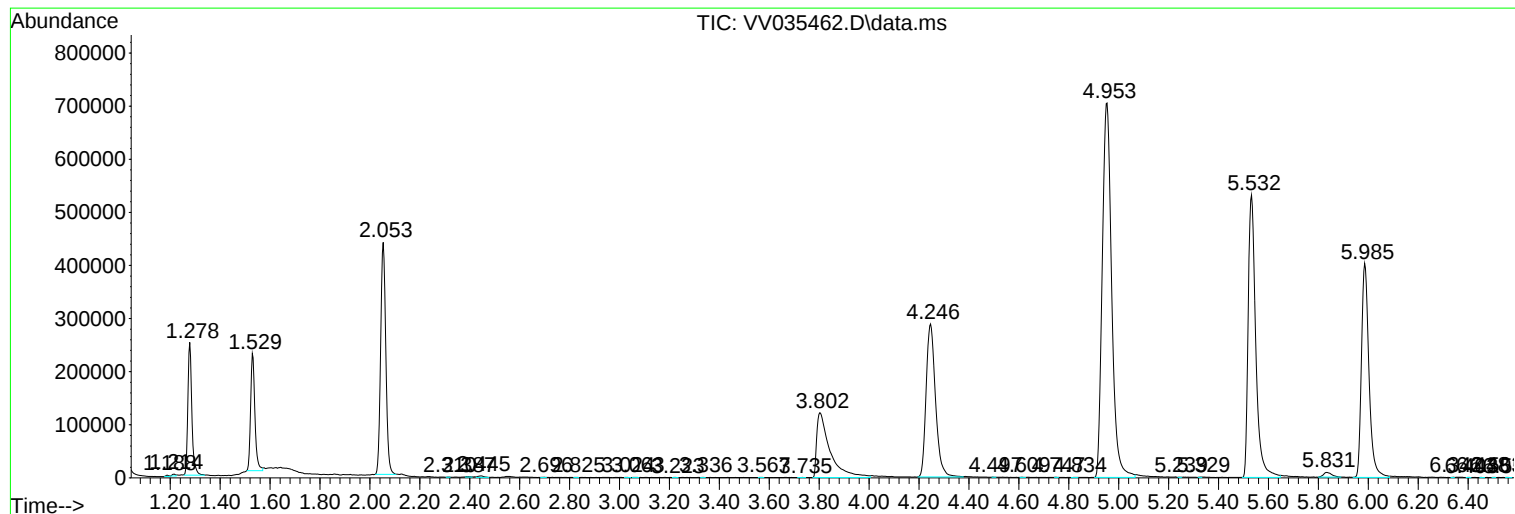

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
Data File : VV035462.D
Acq On : 29 Apr 2024 11:47
Operator : SY/MD
Sample : P2204-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
Data File : VV035462.D
Acq On : 29 Apr 2024 11:47
Operator : SY/MD
Sample : P2204-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------