

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
 Data File : VV035464.D
 Acq On : 29 Apr 2024 12:33
 Operator : SY/MD
 Sample : P2279-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RQ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035464.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.185	41	45	49	rBV	3118	3073	0.04%	0.014%
2	1.214	49	54	61	rVV	10397	12279	0.18%	0.056%
3	1.278	67	74	91	rVB	250595	269235	3.84%	1.223%
4	1.526	145	151	163	rBV	183049	204118	2.91%	0.927%
5	2.053	305	315	333	rBV	423736	617646	8.81%	2.806%
6	2.272	381	383	386	rBV4	451	255	0.00%	0.001%
7	2.298	388	391	396	rVB4	644	544	0.01%	0.002%
8	2.401	420	423	429	rBV4	404	348	0.00%	0.002%
9	2.446	431	437	447	rVB7	1853	3129	0.04%	0.014%
10	2.558	459	472	482	rBV2	18818	44140	0.63%	0.201%
11	2.677	507	509	512	rBV3	419	305	0.00%	0.001%
12	2.857	562	565	572	rVB2	375	425	0.01%	0.002%
13	2.892	572	576	578	rBV2	515	293	0.00%	0.001%
14	2.982	600	604	609	rVB2	438	430	0.01%	0.002%
15	3.034	617	620	627	rVB2	454	462	0.01%	0.002%
16	3.069	627	631	633	rBV	314	240	0.00%	0.001%
17	3.172	660	663	667	rVB2	407	325	0.00%	0.001%
18	3.346	714	717	724	rBV3	230	255	0.00%	0.001%
19	3.542	772	778	783	rVB	296	277	0.00%	0.001%
20	3.671	816	818	822	rVB3	399	322	0.00%	0.001%
21	3.799	848	858	906	rBV	123909	426936	6.09%	1.939%
22	4.246	980	997	1030	rBV	281143	726319	10.36%	3.299%
23	4.487	1070	1072	1076	rBV2	342	236	0.00%	0.001%
24	4.532	1082	1086	1089	rBV3	356	284	0.00%	0.001%
25	4.719	1141	1144	1149	rVB3	422	312	0.00%	0.001%
26	4.809	1165	1172	1174	rBV2	532	617	0.01%	0.003%
27	4.953	1200	1217	1268	rBV2	694393	1817463	25.93%	8.256%
28	5.208	1291	1296	1305	rVB5	895	1488	0.02%	0.007%
29	5.246	1305	1308	1312	rVB3	715	400	0.01%	0.002%
30	5.391	1349	1353	1358	rBV2	379	401	0.01%	0.002%
31	5.439	1363	1368	1376	rVB4	448	490	0.01%	0.002%
32	5.532	1385	1397	1442	rBV	558598	1180163	16.84%	5.361%
33	5.732	1457	1459	1461	rVB	789	372	0.01%	0.002%
34	5.841	1482	1493	1509	rVB5	6896	15765	0.22%	0.072%
35	5.986	1525	1538	1570	rBV	389912	814221	11.62%	3.699%
36	6.214	1607	1609	1612	rVB3	495	275	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
 Data File : VV035464.D
 Acq On : 29 Apr 2024 12:33
 Operator : SY/MD
 Sample : P2279-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RQ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

37	6.233	1612	1615	1618	rBV3	359	262	0.00%	0.001%
38	6.281	1626	1630	1632	rBV2	546	373	0.01%	0.002%
39	6.580	1720	1723	1728	rVB2	350	314	0.00%	0.001%
40	6.690	1750	1757	1764	rBV3	254	403	0.01%	0.002%
41	6.912	1816	1826	1856	rBV	196740	384839	5.49%	1.748%
42	7.178	1906	1909	1912	rVB2	526	265	0.00%	0.001%
43	7.198	1912	1915	1917	rVB2	410	249	0.00%	0.001%
44	7.243	1917	1929	1955	rBV	784673	1386247	19.78%	6.297%
45	7.555	2016	2026	2058	rBV	134060	261526	3.73%	1.188%
46	7.751	2085	2087	2090	rVB4	506	267	0.00%	0.001%
47	7.815	2106	2107	2111	rVB2	458	254	0.00%	0.001%
48	7.873	2120	2125	2127	rBV3	558	593	0.01%	0.003%
49	8.031	2162	2174	2221	rBV3	350223	833107	11.88%	3.785%
50	8.503	2318	2321	2325	rBV4	352	251	0.00%	0.001%
51	8.561	2334	2339	2345	rVB5	521	699	0.01%	0.003%
52	8.616	2354	2356	2360	rVB3	590	305	0.00%	0.001%
53	8.638	2360	2363	2367	rBV3	453	360	0.01%	0.002%
54	8.809	2396	2416	2462	rBV2	3426119	7009762	100.00%	31.843%
55	9.063	2492	2495	2497	rBV2	723	352	0.01%	0.002%
56	9.175	2528	2530	2533	rBV2	344	258	0.00%	0.001%
57	9.252	2551	2554	2559	rBV5	475	491	0.01%	0.002%
58	9.375	2588	2592	2596	rVB4	553	438	0.01%	0.002%
59	9.484	2621	2626	2628	rBV2	426	388	0.01%	0.002%
60	9.619	2666	2668	2671	rBV	468	367	0.01%	0.002%
61	9.719	2694	2699	2701	rBV3	358	308	0.00%	0.001%
62	9.760	2708	2712	2714	rBV	323	260	0.00%	0.001%
63	9.776	2714	2717	2721	rVV	289	281	0.00%	0.001%
64	9.796	2721	2723	2727	rVV3	730	505	0.01%	0.002%
65	9.815	2727	2729	2733	rVB4	685	497	0.01%	0.002%
66	9.847	2733	2739	2741	rBV3	687	638	0.01%	0.003%
67	9.944	2765	2769	2774	rVB2	708	545	0.01%	0.002%
68	9.979	2774	2780	2781	rBV2	294	327	0.00%	0.001%
69	10.153	2820	2834	2863	rBV	582165	940916	13.42%	4.274%
70	10.256	2863	2866	2871	rVB4	783	669	0.01%	0.003%
71	10.307	2879	2882	2884	rBV2	344	252	0.00%	0.001%
72	10.407	2910	2913	2917	rBV2	317	260	0.00%	0.001%
73	10.484	2934	2937	2939	rBV2	451	260	0.00%	0.001%
74	10.580	2964	2967	2972	rVV2	388	289	0.00%	0.001%
75	10.786	3029	3031	3035	rVV2	516	307	0.00%	0.001%
76	11.075	3117	3121	3123	rBV2	323	236	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
 Data File : VV035464.D
 Acq On : 29 Apr 2024 12:33
 Operator : SY/MD
 Sample : P2279-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RQ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

77	11.120	3123	3135	3144	rBV	54388	89626	1.28%	0.407%
78	11.185	3144	3155	3189	rVB2	886125	2224265	31.73%	10.104%
79	11.391	3217	3219	3225	rVB5	1198	717	0.01%	0.003%
80	11.567	3256	3274	3305	rBV2	1110406	2647522	37.77%	12.027%
81	11.802	3345	3347	3351	rVB3	777	530	0.01%	0.002%
82	11.821	3351	3353	3356	rBV2	547	263	0.00%	0.001%
83	11.860	3363	3365	3368	rBV3	528	386	0.01%	0.002%
84	11.950	3391	3393	3397	rBV2	400	277	0.00%	0.001%
85	12.043	3416	3422	3425	rVB3	452	504	0.01%	0.002%
86	12.079	3425	3433	3436	rBV3	560	632	0.01%	0.003%
87	12.149	3450	3455	3457	rBV	505	390	0.01%	0.002%
88	12.182	3461	3465	3466	rBV2	426	336	0.00%	0.002%
89	12.339	3511	3514	3516	rBV	611	388	0.01%	0.002%
90	12.812	3656	3661	3662	rBV2	496	334	0.00%	0.002%
91	12.825	3662	3665	3669	rVB2	457	335	0.00%	0.002%
92	12.892	3683	3686	3691	rBV2	535	340	0.00%	0.002%
93	12.947	3699	3703	3706	rBV2	348	296	0.00%	0.001%
94	13.085	3743	3746	3748	rBV	430	331	0.00%	0.002%
95	13.201	3772	3782	3796	rBV3	35900	60824	0.87%	0.276%
96	13.455	3854	3861	3869	rBV3	2636	3568	0.05%	0.016%
97	13.686	3925	3933	3943	rBV3	5405	8083	0.12%	0.037%
98	13.863	3985	3988	3991	rBV2	405	271	0.00%	0.001%
99	13.985	4024	4026	4030	rBV3	375	249	0.00%	0.001%
100	14.828	4286	4288	4291	rBV3	619	347	0.00%	0.002%




Sum of corrected areas: 22013577

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
Data File : VV035464.D
Acq On : 29 Apr 2024 12:33
Operator : SY/MD
Sample : P2279-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RQ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

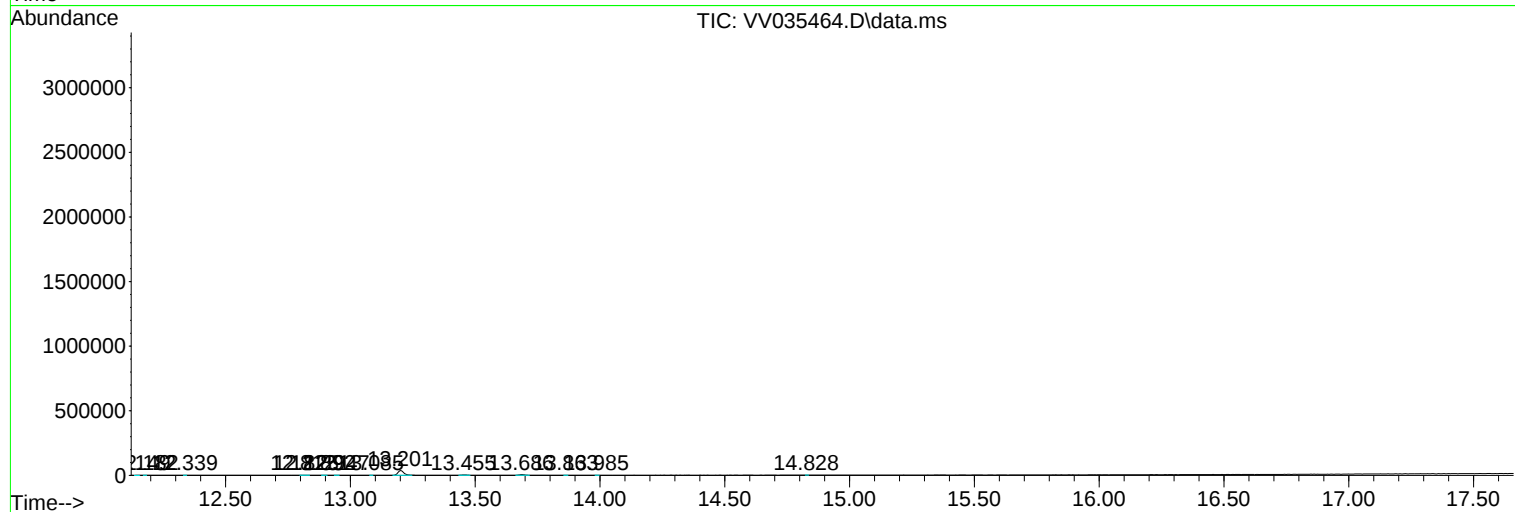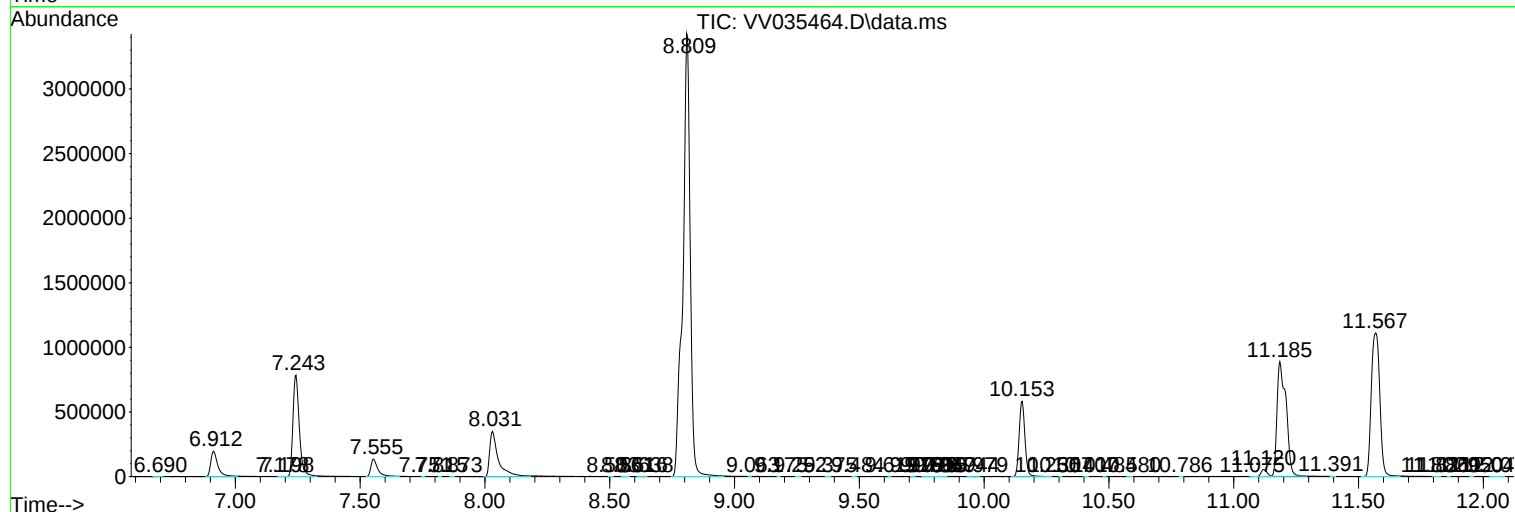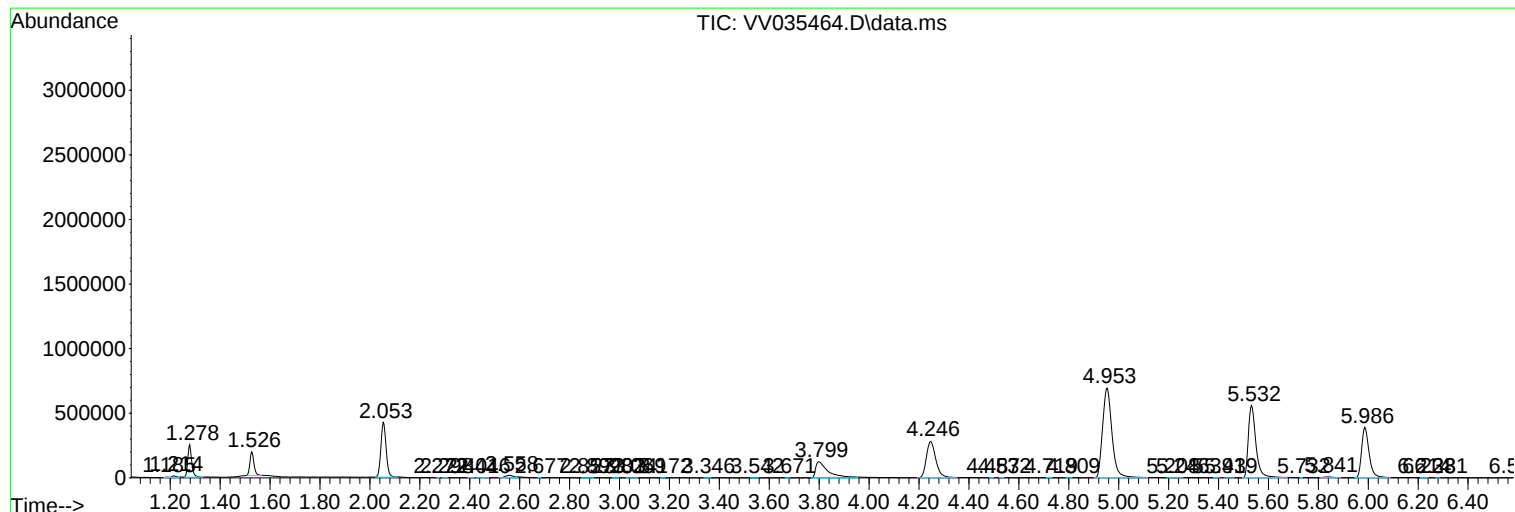

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
Data File : VV035464.D
Acq On : 29 Apr 2024 12:33
Operator : SY/MD
Sample : P2279-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RQ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
Data File : VV035464.D
Acq On : 29 Apr 2024 12:33
Operator : SY/MD
Sample : P2279-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RQ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc