

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
 Data File : VV035465.D
 Acq On : 29 Apr 2024 12:57
 Operator : SY/MD
 Sample : P2269-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RP7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035465.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.188	41	46	48	rBV	2298	1998	0.04%	0.010%
2	1.214	49	54	62	rVV	10815	13430	0.27%	0.066%
3	1.278	67	74	89	rVV	250775	277664	5.55%	1.361%
4	1.529	145	152	165	rBV	199797	231313	4.63%	1.134%
5	2.053	305	315	329	rBV	437894	629232	12.58%	3.085%
6	2.130	332	339	361	rVB	25170	57144	1.14%	0.280%
7	2.301	390	392	396	rBV3	549	408	0.01%	0.002%
8	2.555	458	471	482	rBV	30051	67203	1.34%	0.330%
9	2.770	536	538	543	rVB2	291	208	0.00%	0.001%
10	2.867	564	568	575	rBV	324	243	0.00%	0.001%
11	2.931	584	588	593	rBV3	356	317	0.01%	0.002%
12	3.024	614	617	624	rVB	339	311	0.01%	0.002%
13	3.069	624	631	633	rBV3	308	333	0.01%	0.002%
14	3.143	651	654	657	rBV2	322	255	0.01%	0.001%
15	3.204	670	673	676	rBV2	415	281	0.01%	0.001%
16	3.220	676	678	686	rVB2	430	341	0.01%	0.002%
17	3.256	686	689	694	rBV3	261	233	0.00%	0.001%
18	3.278	694	696	699	rBV	284	239	0.00%	0.001%
19	3.802	844	859	916	rBV	122883	477050	9.54%	2.339%
20	4.246	981	997	1033	rBV	282935	728970	14.58%	3.574%
21	4.455	1059	1062	1066	rVB4	718	543	0.01%	0.003%
22	4.503	1074	1077	1081	rBV3	420	309	0.01%	0.002%
23	4.953	1201	1217	1267	rBV2	699413	1863715	37.28%	9.139%
24	5.291	1316	1322	1324	rBV4	440	430	0.01%	0.002%
25	5.339	1332	1337	1342	rBV5	557	571	0.01%	0.003%
26	5.375	1346	1348	1352	rVB2	562	272	0.01%	0.001%
27	5.429	1361	1365	1369	rBV4	425	446	0.01%	0.002%
28	5.532	1386	1397	1442	rBV	564756	1189026	23.78%	5.830%
29	5.754	1464	1466	1467	rBV2	494	246	0.00%	0.001%
30	5.834	1481	1491	1509	rVB3	9746	19849	0.40%	0.097%
31	5.934	1517	1522	1524	rBV3	442	362	0.01%	0.002%
32	5.985	1525	1538	1577	rVV	389157	818412	16.37%	4.013%
33	6.272	1624	1627	1630	rBV4	347	245	0.00%	0.001%
34	6.288	1630	1632	1634	rVB2	409	209	0.00%	0.001%
35	6.384	1657	1662	1665	rBV2	271	218	0.00%	0.001%
36	6.500	1694	1698	1702	rVV	268	229	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042924\
 Data File : VW035465.D
 Acq On : 29 Apr 2024 12:57
 Operator : SY/MD
 Sample : P2269-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RP7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

37	6.548	1707	1713	1716	rBV3	325	271	0.01%	0.001%
38	6.596	1724	1728	1732	rVB2	397	324	0.01%	0.002%
39	6.815	1794	1796	1801	rVB2	423	339	0.01%	0.002%
40	6.911	1816	1826	1861	rBV	200029	389844	7.80%	1.912%
41	7.117	1888	1890	1895	rVB2	399	293	0.01%	0.001%
42	7.194	1912	1914	1918	rVB2	798	526	0.01%	0.003%
43	7.243	1918	1929	1964	rBV	788560	1408928	28.18%	6.909%
44	7.555	2016	2026	2052	rBV	136031	258550	5.17%	1.268%
45	7.850	2114	2118	2122	rBV4	402	417	0.01%	0.002%
46	7.924	2139	2141	2150	rVB4	712	572	0.01%	0.003%
47	8.034	2162	2175	2219	rBV2	355201	854142	17.08%	4.188%
48	8.429	2295	2298	2304	rBV5	691	747	0.01%	0.004%
49	8.464	2307	2309	2312	rVB	533	267	0.01%	0.001%
50	8.606	2348	2353	2358	rBV4	401	473	0.01%	0.002%
51	8.632	2358	2361	2363	rVB2	358	213	0.00%	0.001%
52	8.651	2363	2367	2371	rBV2	468	414	0.01%	0.002%
53	8.706	2380	2384	2387	rBV3	286	244	0.00%	0.001%
54	8.783	2397	2408	2442	rBV2	906596	1963059	39.26%	9.626%
55	9.133	2514	2517	2521	rVB2	556	421	0.01%	0.002%
56	9.162	2521	2526	2527	rBV3	378	278	0.01%	0.001%
57	9.207	2537	2540	2542	rBV3	534	361	0.01%	0.002%
58	9.220	2542	2544	2550	rVB2	471	443	0.01%	0.002%
59	9.268	2556	2559	2562	rBV	336	206	0.00%	0.001%
60	9.432	2607	2610	2612	rBV	471	248	0.00%	0.001%
61	9.445	2612	2614	2619	rVB2	526	284	0.01%	0.001%
62	9.484	2619	2626	2627	rBV3	345	355	0.01%	0.002%
63	9.538	2640	2643	2648	rBV3	356	319	0.01%	0.002%
64	9.561	2648	2650	2654	rVB	361	224	0.00%	0.001%
65	9.596	2654	2661	2663	rBV2	362	422	0.01%	0.002%
66	9.805	2723	2726	2729	rBV2	232	207	0.00%	0.001%
67	9.844	2735	2738	2742	rBV2	346	373	0.01%	0.002%
68	9.982	2775	2781	2783	rVV3	261	226	0.00%	0.001%
69	10.043	2798	2800	2805	rVB	380	271	0.01%	0.001%
70	10.072	2806	2809	2814	rVB2	305	214	0.00%	0.001%
71	10.152	2822	2834	2861	rBV	601075	956393	19.13%	4.690%
72	10.310	2880	2883	2884	rBV2	331	208	0.00%	0.001%
73	10.468	2929	2932	2937	rVB2	281	228	0.00%	0.001%
74	10.564	2960	2962	2967	rVB	380	216	0.00%	0.001%
75	10.686	2996	3000	3003	rBV2	543	453	0.01%	0.002%
76	10.709	3003	3007	3012	rVB2	343	333	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
 Data File : VV035465.D
 Acq On : 29 Apr 2024 12:57
 Operator : SY/MD
 Sample : P2269-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RP7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

77	10.741	3012	3017	3022	rBB3	423	326	0.01%	0.002%
78	10.789	3029	3032	3037	rVB3	477	383	0.01%	0.002%
79	10.841	3044	3048	3050	rBV	323	247	0.00%	0.001%
80	10.992	3091	3095	3098	rBV3	390	271	0.01%	0.001%
81	11.120	3125	3135	3145	rBV	94774	151376	3.03%	0.742%
82	11.185	3145	3155	3184	rVB2	898024	1649406	32.99%	8.088%
83	11.493	3242	3251	3260	rBV3	16477	34403	0.69%	0.169%
84	11.574	3261	3276	3306	rVB2	2528808	4999888	100.00%	24.516%
85	12.075	3429	3432	3434	rBV2	477	312	0.01%	0.002%
86	12.178	3461	3464	3466	rBV	411	284	0.01%	0.001%
87	12.323	3507	3509	3513	rVB2	628	331	0.01%	0.002%
88	12.358	3518	3520	3525	rVB2	428	306	0.01%	0.002%
89	12.474	3553	3556	3559	rVB2	536	325	0.01%	0.002%
90	12.519	3564	3570	3572	rBV2	485	443	0.01%	0.002%
91	12.580	3580	3589	3605	rBV	39710	74583	1.49%	0.366%
92	12.686	3616	3622	3634	rVB7	3264	5651	0.11%	0.028%
93	12.770	3645	3648	3653	rBV3	383	337	0.01%	0.002%
94	12.850	3671	3673	3676	rBV3	389	221	0.00%	0.001%
95	13.197	3769	3781	3809	rBV	501343	793434	15.87%	3.891%
96	13.451	3855	3860	3870	rVB4	3368	5217	0.10%	0.026%
97	13.680	3920	3931	3958	rBV	227260	374223	7.48%	1.835%
98	14.094	4052	4060	4079	rBV4	9034	20813	0.42%	0.102%
99	14.760	4257	4267	4278	rBV3	8422	14338	0.29%	0.070%
100	15.332	4437	4445	4457	rBV3	27276	42399	0.85%	0.208%




Sum of corrected areas: 20394078

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
Data File : VV035465.D
Acq On : 29 Apr 2024 12:57
Operator : SY/MD
Sample : P2269-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RP7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

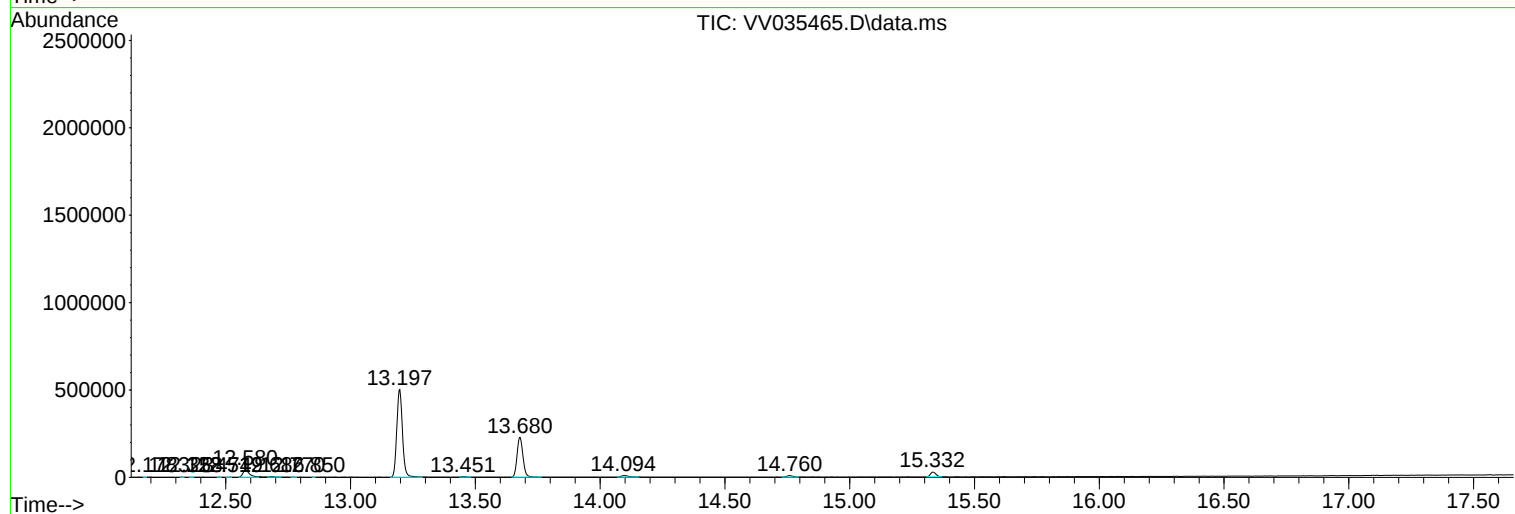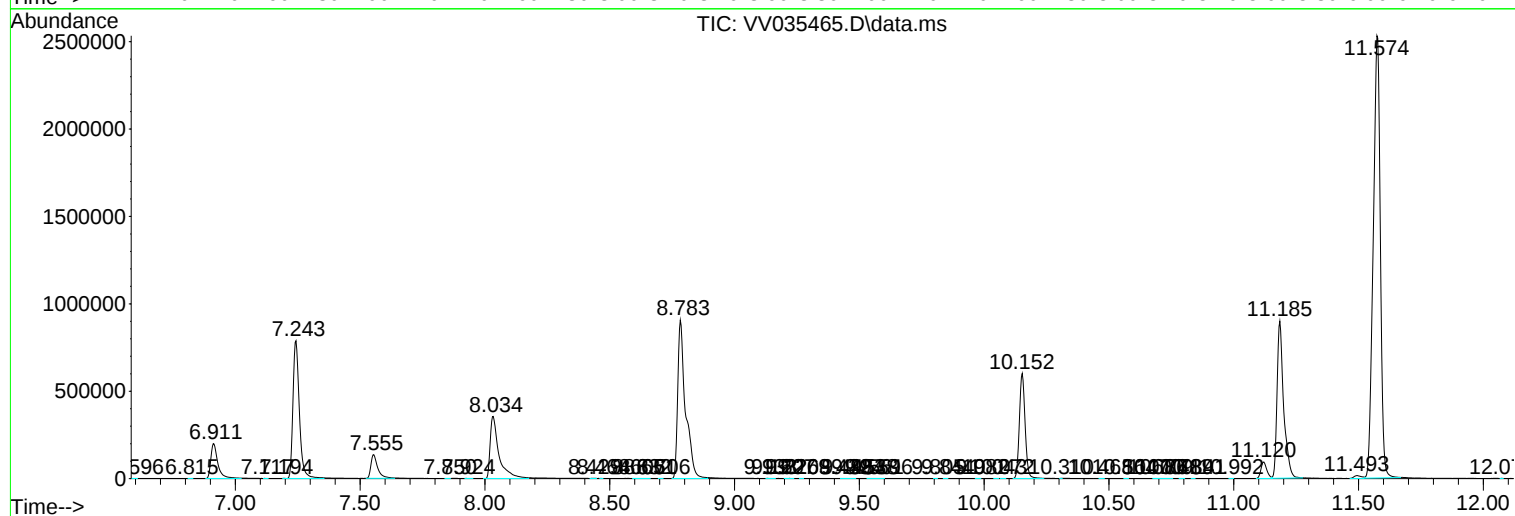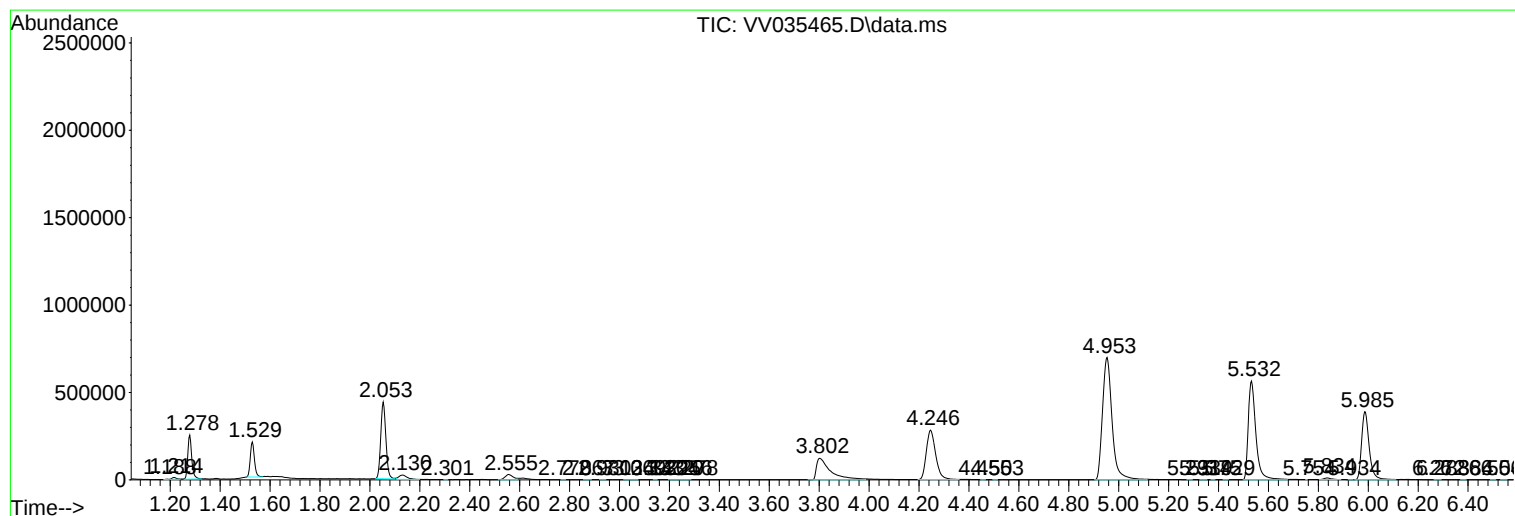

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
Data File : VV035465.D
Acq On : 29 Apr 2024 12:57
Operator : SY/MD
Sample : P2269-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RP7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
Data File : VV035465.D
Acq On : 29 Apr 2024 12:57
Operator : SY/MD
Sample : P2269-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RP7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------